


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
 Data File : VU047356.D
 Acq On : 07 Mar 2022 08:55
 Operator : SY/MD
 Sample : BFB062
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB062

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Mar 04 23:20:39 2022

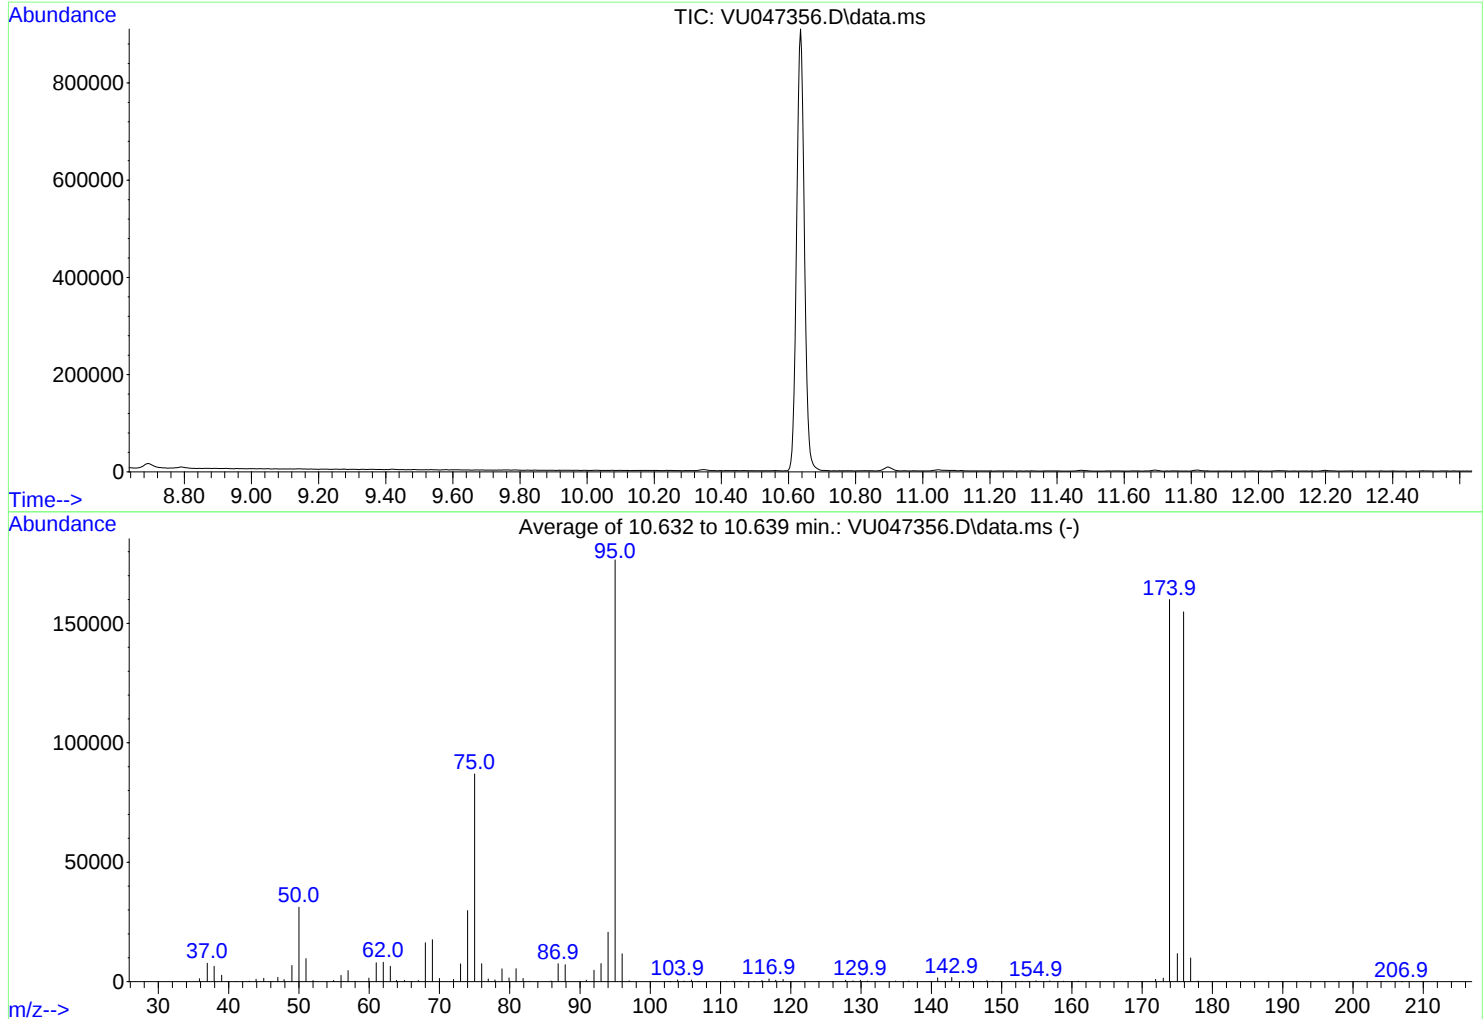

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	31149	PASS
75	95	30	80	49.2	86939	PASS
95	95	100	100	100.0	176619	PASS
96	95	5	9	6.6	11657	PASS
173	174	0.00	2	0.9	1488	PASS
174	95	50	120	90.6	160000	PASS
175	174	5	9	7.3	11728	PASS
176	174	95	101	96.8	154837	PASS
177	176	5	9	6.4	9896	PASS

m/z	Abundance
35.90	1236.0
36.90	115.0
37.90	503.0
39.90	247.0
43.90	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB062

m/z	Abundance
35.90	2357.0
37.00	7715.0
38.00	7014.0
39.00	2734.0
39.90	331.0
42.90	226.0
43.90	1230.0
45.00	1394.0
45.90	119.0
47.00	1778.0
47.90	863.0
49.00	6822.0
50.00	31232.0
51.00	9726.0
52.00	461.0
54.90	534.0
56.00	2687.0
57.00	4600.0
58.00	182.0
60.00	1583.0
61.00	8038.0
62.00	8081.0
63.00	6617.0
63.90	627.0
65.00	605.0
67.00	448.0
68.00	16504.0
69.00	17488.0
70.00	1320.0
72.00	900.0
73.00	7488.0
74.00	29800.0
75.00	86904.0
76.00	7552.0
77.00	1228.0
77.90	722.0
78.90	5279.0
79.90	1596.0
80.90	5360.0
81.90	1297.0
82.90	149.0
85.90	263.0
86.90	7337.0
87.90	7051.0
90.90	555.0
92.00	4619.0
93.00	7513.0
94.00	20480.0
95.00	175232.0
96.00	11963.0
97.00	360.0
103.90	782.0
104.80	267.0
105.80	673.0
106.90	164.0
109.90	151.0
110.80	150.0
111.80	163.0
112.80	157.0
114.80	168.0
115.90	536.0
116.90	1141.0
117.80	641.0
118.90	939.0
127.80	640.0
128.90	316.0
129.90	593.0
130.90	236.0
134.90	286.0
136.80	285.0
140.90	1537.0
141.90	169.0
142.90	1724.0
144.90	143.0
145.90	215.0
146.90	126.0
147.90	435.0
148.80	156.0
149.80	137.0
152.90	111.0
153.80	101.0
154.90	377.0
156.90	300.0
158.80	206.0
160.90	201.0
171.90	1003.0
173.00	1498.0
173.90	155456.0
175.00	11351.0
175.90	148800.0
176.90	9884.0
178.00	241.0

Instrument :
MSVOA_U
ClientSampleId :
BFB062

m/z	Abundance
35.90	2441.0
37.00	8108.0
38.00	7156.0
39.00	2823.0
40.00	354.0
41.00	112.0
43.00	218.0
43.90	1305.0
45.00	1438.0
46.20	100.0
47.00	1850.0
47.90	848.0
49.00	7011.0
50.00	32152.0
51.00	9964.0
52.00	504.0
55.00	591.0
56.00	2755.0
57.00	4769.0
58.00	227.0
59.90	1539.0
61.00	8196.0
62.00	8440.0
63.00	6656.0
63.90	556.0
65.00	551.0
67.00	453.0
68.00	16784.0
69.00	18152.0
70.00	1407.0
72.00	945.0
73.00	7654.0
74.00	30672.0
75.00	89816.0
76.00	7809.0
77.00	1186.0
77.90	780.0
78.90	5492.0
79.90	1620.0
80.90	5597.0
81.90	1391.0
82.80	149.0
85.90	269.0
86.90	7781.0
87.90	7386.0
90.90	655.0
92.00	4891.0
93.00	7818.0
94.00	21280.0
95.00	182464.0
96.00	11970.0
97.00	327.0
102.80	100.0
103.90	788.0
104.80	282.0
105.90	691.0
106.90	164.0
109.90	146.0
110.80	129.0
111.80	197.0
112.80	150.0
114.80	166.0
115.90	542.0
116.90	1166.0
117.90	661.0
118.90	1015.0
123.90	102.0
127.80	645.0
128.80	334.0
129.90	657.0
130.90	248.0
134.90	284.0
136.80	309.0
139.80	115.0
140.90	1658.0
141.90	164.0
142.90	1789.0
144.80	149.0
145.80	251.0
146.90	130.0
147.90	395.0
148.70	156.0
149.80	144.0
152.90	125.0
153.80	146.0
154.90	442.0
156.80	355.0
158.80	213.0
160.90	201.0
171.90	972.0
173.00	1540.0
173.90	165120.0

Instrument :
MSVOA_U
ClientSampleId :
BFB062

175.00	12151.0
175.90	160128.0
176.90	10151.0
178.00	246.0

Instrument :
MSVOA_U
ClientSampleId :
BFB062

m/z	Abundance
35.90	2490.0
37.00	7661.0
38.00	6669.0
39.00	2595.0
40.00	334.0
41.00	110.0
42.90	183.0
43.90	1259.0
45.00	1395.0
46.20	105.0
47.00	1732.0
47.90	845.0
49.00	6410.0
50.00	30064.0
51.00	9189.0
52.00	477.0
55.00	570.0
56.00	2488.0
57.00	4433.0
58.00	232.0
60.00	1375.0
61.00	7592.0
62.00	7830.0
63.00	6089.0
63.90	459.0
65.00	459.0
66.00	104.0
67.00	431.0
68.00	15508.0
69.00	17048.0
70.00	1332.0
72.00	908.0
73.00	7237.0
74.00	28760.0
75.00	84096.0
76.00	7222.0
76.90	995.0
77.90	786.0
78.90	5251.0
79.90	1523.0
80.90	5310.0
81.90	1342.0
82.80	147.0
85.90	244.0
86.90	7425.0
87.90	6893.0
90.90	706.0
92.00	4725.0
93.00	7318.0
94.00	20320.0
95.00	172160.0
96.00	11038.0
97.00	268.0
103.90	756.0
104.80	272.0
105.90	645.0
106.90	147.0
110.00	107.0
110.90	109.0
111.80	174.0
113.00	141.0
114.80	156.0
115.90	480.0
116.90	1063.0
117.90	610.0
118.90	953.0
123.90	114.0
125.90	107.0
127.80	582.0
128.80	292.0
129.90	629.0
130.90	251.0
134.90	285.0
136.80	289.0
139.90	113.0
140.90	1595.0
141.90	153.0
142.90	1648.0
144.80	146.0
145.80	268.0
146.90	110.0
147.90	371.0
148.70	137.0
149.90	143.0
152.90	138.0
153.80	165.0
154.90	469.0
156.80	352.0
158.80	223.0
160.90	168.0
171.90	856.0
173.00	1425.0

Instrument :
MSVOA_U
ClientSampleId :
BFB062

173.90	159424.0
175.00	11683.0
175.90	155584.0
176.90	9652.0
177.90	242.0
206.90	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB062