

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030822\
 Data File : VU047383.D
 Acq On : 08 Mar 2022 11:57
 Operator : SY/MD
 Sample : N1773-10DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFY17DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047383.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	97	rVB	55683	64588	7.80%	1.065%
2	1.919	170	180	196	rBV	55258	77495	9.36%	1.278%
3	2.575	371	384	400	rBV2	102161	174413	21.06%	2.877%
4	4.642	1010	1027	1063	rBV2	86186	350437	42.32%	5.781%
5	5.070	1143	1160	1186	rVB	110660	244074	29.47%	4.026%
6	5.729	1343	1365	1385	rBV2	206470	548404	66.22%	9.047%
7	6.253	1514	1528	1548	rBV	207471	392878	47.44%	6.481%
8	6.546	1605	1619	1636	rBV	264310	489802	59.14%	8.080%
9	6.694	1652	1665	1682	rBV	137734	266881	32.23%	4.403%
10	7.568	1923	1937	1954	rBV	73421	127945	15.45%	2.111%
11	7.899	2024	2040	2061	rBV	238995	422397	51.00%	6.968%
12	8.182	2117	2128	2142	rBV	47243	80297	9.70%	1.325%
13	8.555	2232	2244	2257	rBV	169949	284642	34.37%	4.696%
14	8.639	2257	2270	2309	rVV	408632	828162	100.00%	13.662%
15	8.790	2309	2317	2329	rVB3	5548	9766	1.18%	0.161%
16	9.420	2500	2513	2541	rBV	294388	490279	59.20%	8.088%
17	10.758	2915	2929	2943	rBV	137331	224097	27.06%	3.697%
18	11.812	3245	3257	3277	rBV	334134	528299	63.79%	8.715%
19	12.195	3364	3376	3392	rBV	285745	457073	55.19%	7.540%




Sum of corrected areas: 6061929

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030822\
Data File : VU047383.D
Acq On : 08 Mar 2022 11:57
Operator : SY/MD
Sample : N1773-10DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFY17DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

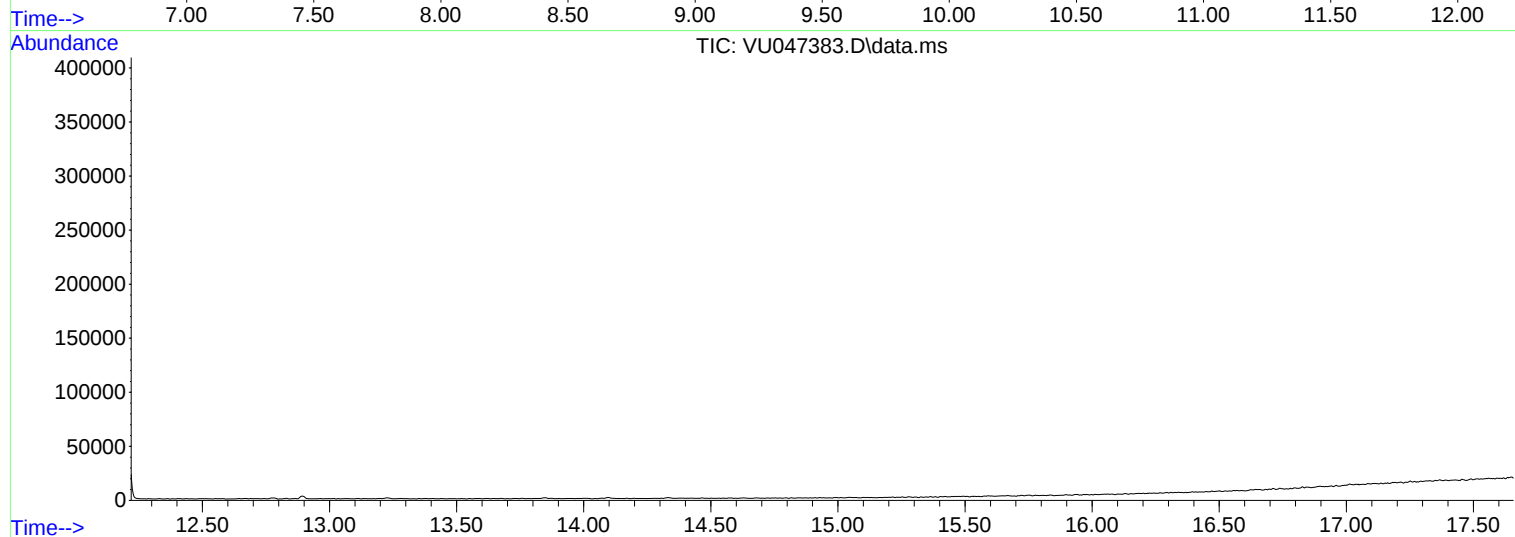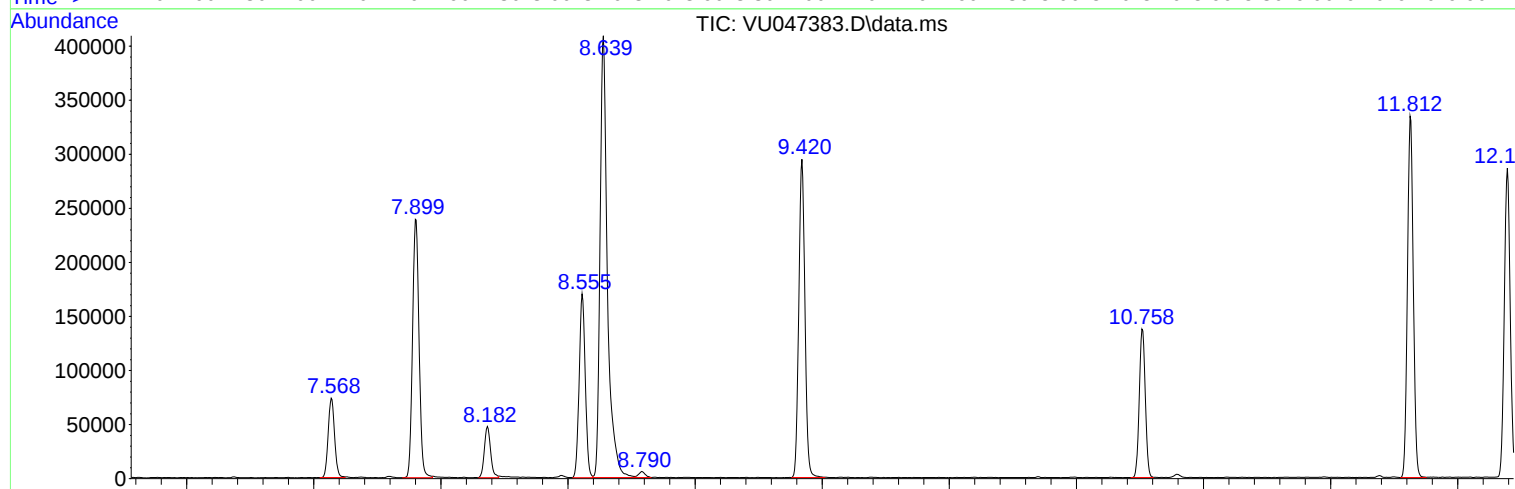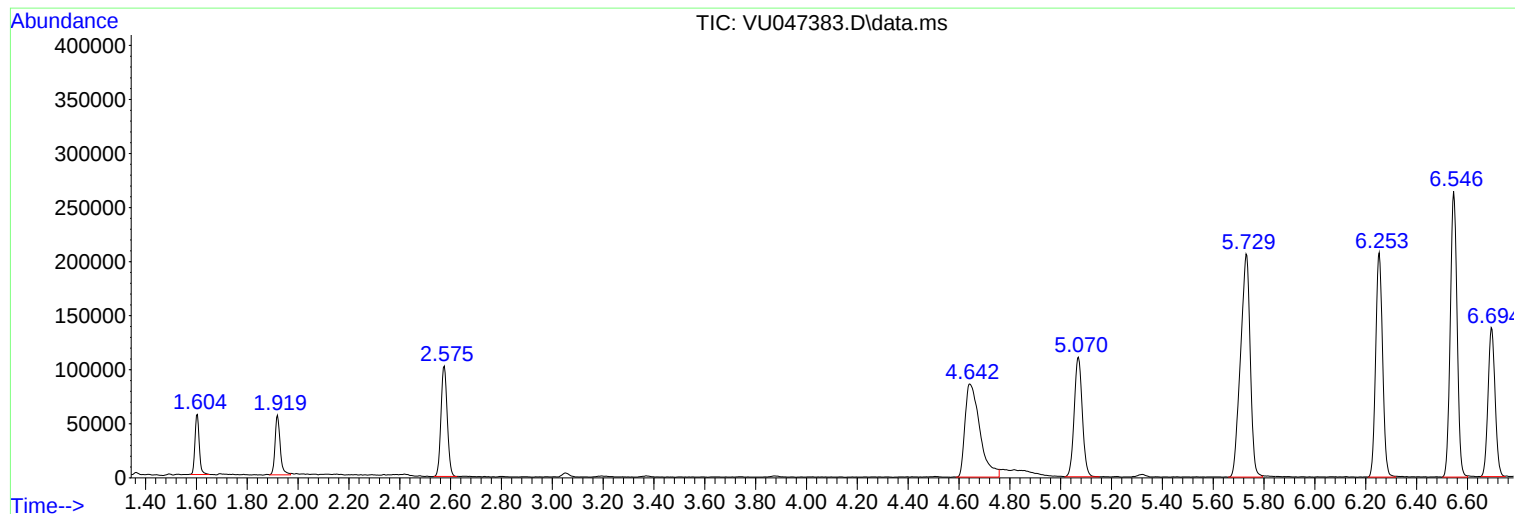

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030822\
Data File : VU047383.D
Acq On : 08 Mar 2022 11:57
Operator : SY/MD
Sample : N1773-10DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFY17DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030822\
Data File : VU047383.D
Acq On : 08 Mar 2022 11:57
Operator : SY/MD
Sample : N1773-10DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFY17DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc