
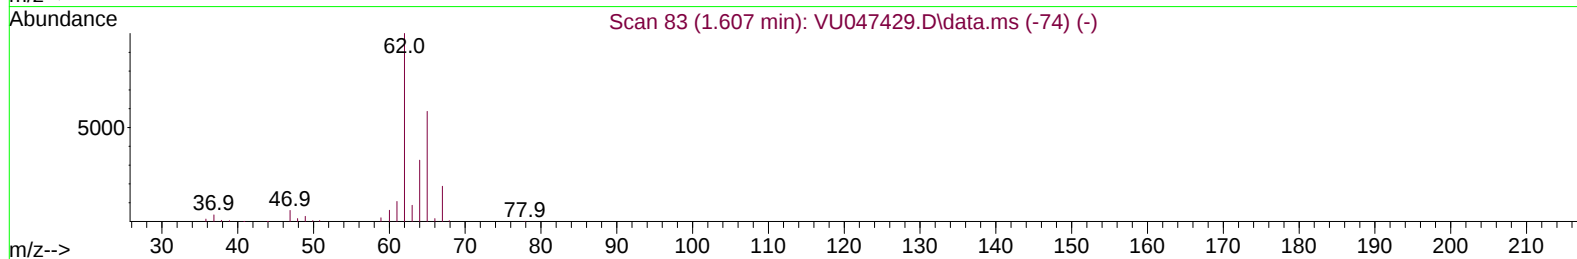
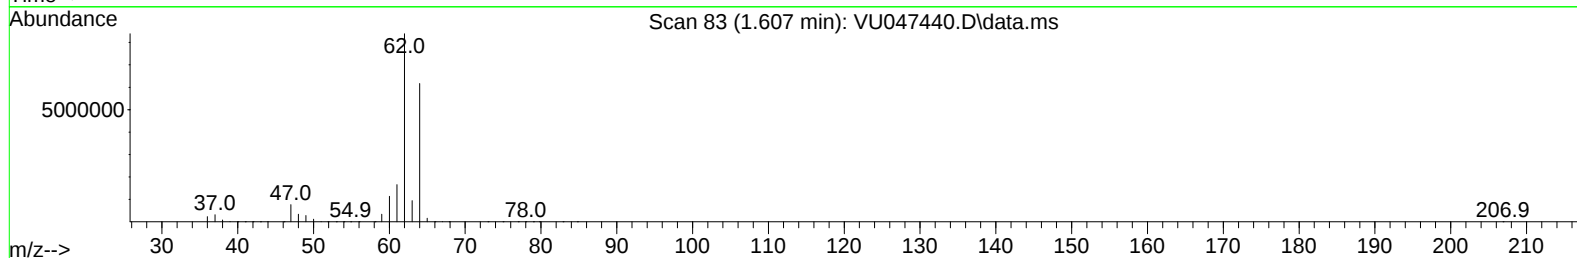


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030922\
Data File : VU047440.D
Acq On : 10 Mar 2022 06:53
Operator : SY/MD
Sample : N1857-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Quant Time: Mar 10 07:49:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 10 03:57:44 2022
Response via : Initial Calibration

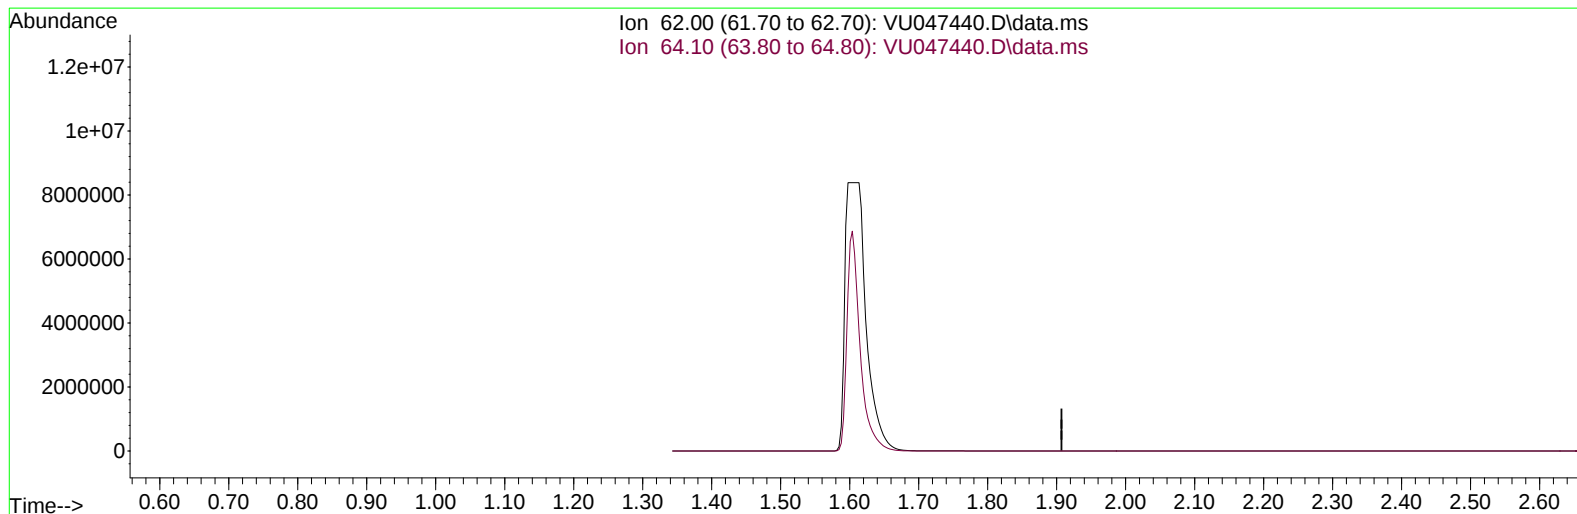

TIC: VU047440.D\data.ms

(5) Vinyl chloride (T)

1.607min (-1.607) 0.00 ug/L

response 0

Ion	Exp%	Act%
62.00	100.00	0.00
64.10	33.80	0.00#
0.00	0.00	0.00
0.00	0.00	0.00