

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030922\
 Data File : VU047425.D
 Acq On : 09 Mar 2022 23:27
 Operator : SY/MD
 Sample : N1861-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YATM3

Quant Time: Mar 10 01:09:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 10 00:51:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	169974	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	161871	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	86954	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	44832	4.863	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.200%
7) Chloroethane-d5	1.919	69	33399	4.935	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.800%
11) 1,1-Dichloroethene-d2	2.575	65	20372	5.003	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	100.000%
20) 2-Butanone-d5	4.645	46	87281	53.178	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.360%
24) Chloroform-d	5.067	84	70168	4.778	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
26) 1,2-Dichloroethane-d4	5.706	65	36361	4.889	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.800%
32) Benzene-d6	5.732	84	153451	5.040	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.800%
36) 1,2-Dichloropropane-d6	6.694	67	45539	5.056	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.200%
41) Toluene-d8	7.899	98	145028	4.846	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.000%
43) trans-1,3-Dichloroprop...	8.182	79	18405	4.813	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.200%
46) 2-Hexanone-d5	8.639	63	85843	50.954	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.900%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	37672	4.799	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.000%
66) 1,2-Dichlorobenzene-d4	12.195	152	56268	5.104	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.000%
Target Compounds					Qvalue	
33) Benzene	5.774	78	7669	0.175	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030922\
Data File : VU047425.D
Acq On : 09 Mar 2022 23:27
Operator : SY/MD
Sample : N1861-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YATM3

Quant Time: Mar 10 01:09:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 10 00:51:00 2022
Response via : Initial Calibration

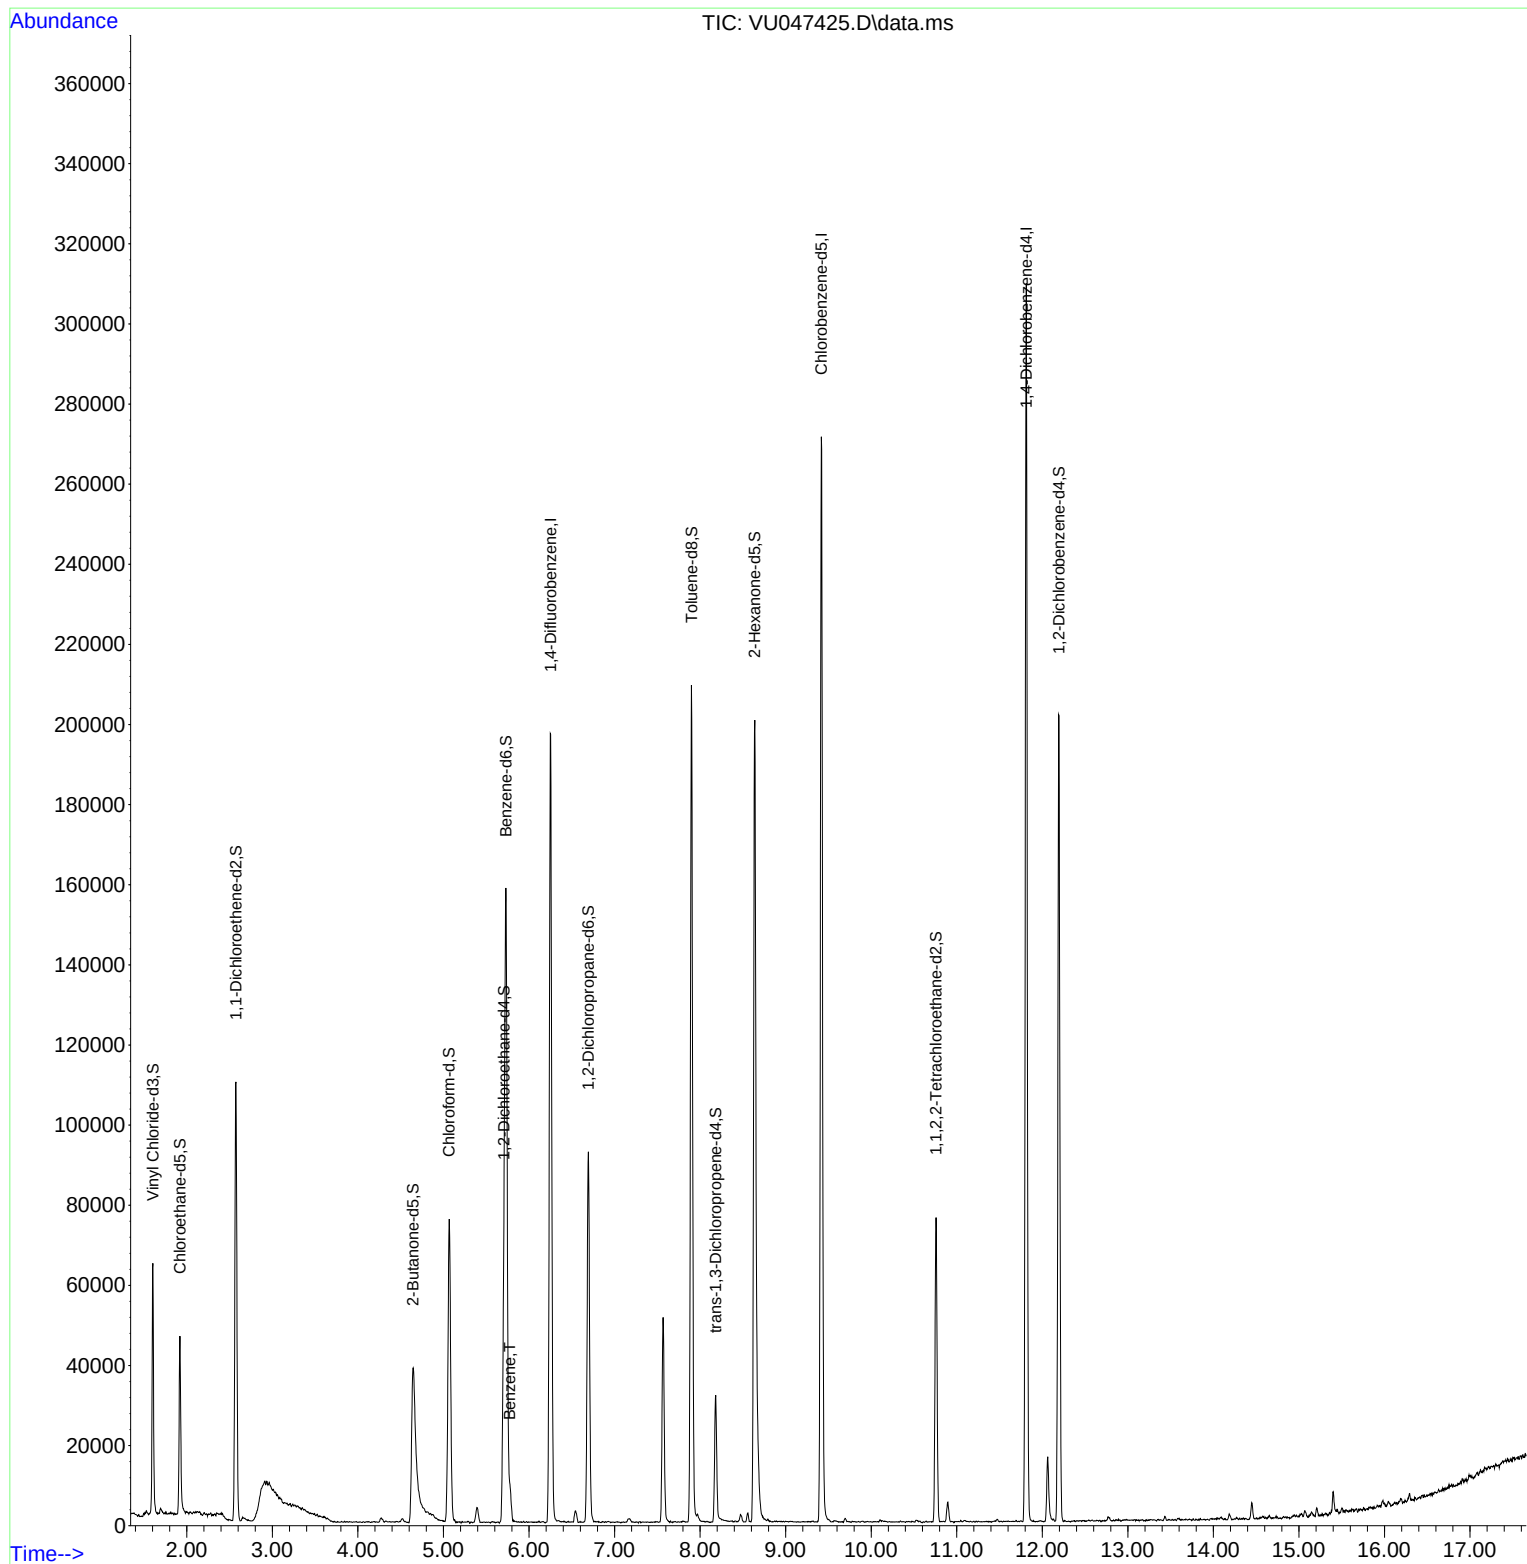

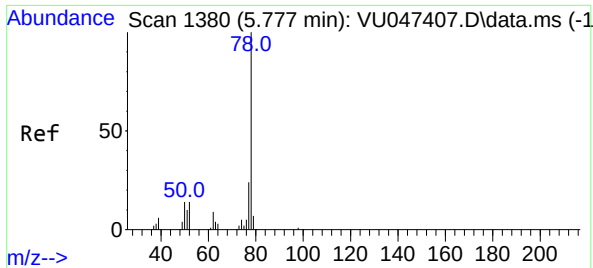

#33
Benzene
Concen: 0.175 ug/L
RT: 5.774 min Scan# 11
Delta R.T. -0.003 min
Lab File: VU047425.D
Acq: 09 Mar 2022 23:27

Instrument :
MSVOA_U
ClientSampleId :
YATM3

Tgt Ion: 78 Resp: 7669

