

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030922\
 Data File : VU047422.D
 Acq On : 09 Mar 2022 22:17
 Operator : SY/MD
 Sample : N1861-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YATMO

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	69	81	96	rBV	63012	77771	3.69%	1.117%
2	1.919	171	180	192	rBV	43876	59037	2.80%	0.848%
3	2.575	369	384	397	rBV2	114625	195306	9.26%	2.806%
4	2.658	397	410	442	rVV2	22403	81925	3.88%	1.177%
5	2.893	452	483	484	rBV6	14850	51578	2.45%	0.741%
6	4.645	1013	1028	1061	rBV	40528	146614	6.95%	2.107%
7	5.070	1144	1160	1183	rVB	77280	184682	8.76%	2.654%
8	5.729	1344	1365	1390	rBV2	159245	406414	19.27%	5.839%
9	6.250	1512	1527	1546	rBV	202563	384833	18.25%	5.529%
10	6.546	1603	1619	1646	rBV	1123757	2108977	100.00%	30.302%
11	6.693	1652	1665	1681	rVB	93212	182458	8.65%	2.622%
12	7.568	1925	1937	1957	rBV	51499	90184	4.28%	1.296%
13	7.899	2026	2040	2059	rBV	212050	364324	17.27%	5.235%
14	8.182	2117	2128	2140	rBV	31973	54017	2.56%	0.776%
15	8.555	2231	2244	2258	rBV	411414	694070	32.91%	9.973%
16	8.635	2258	2269	2300	rVB	202556	404768	19.19%	5.816%
17	9.417	2500	2512	2537	rBV	281524	480388	22.78%	6.902%
18	10.758	2917	2929	2945	rBV	77208	123919	5.88%	1.780%
19	11.812	3244	3257	3273	rBV	320081	509308	24.15%	7.318%
20	12.063	3325	3335	3353	rBV2	16529	29712	1.41%	0.427%
21	12.195	3363	3376	3395	rVB	205260	329515	15.62%	4.735%




Sum of corrected areas: 6959800

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030922\
Data File : VU047422.D
Acq On : 09 Mar 2022 22:17
Operator : SY/MD
Sample : N1861-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YATM0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

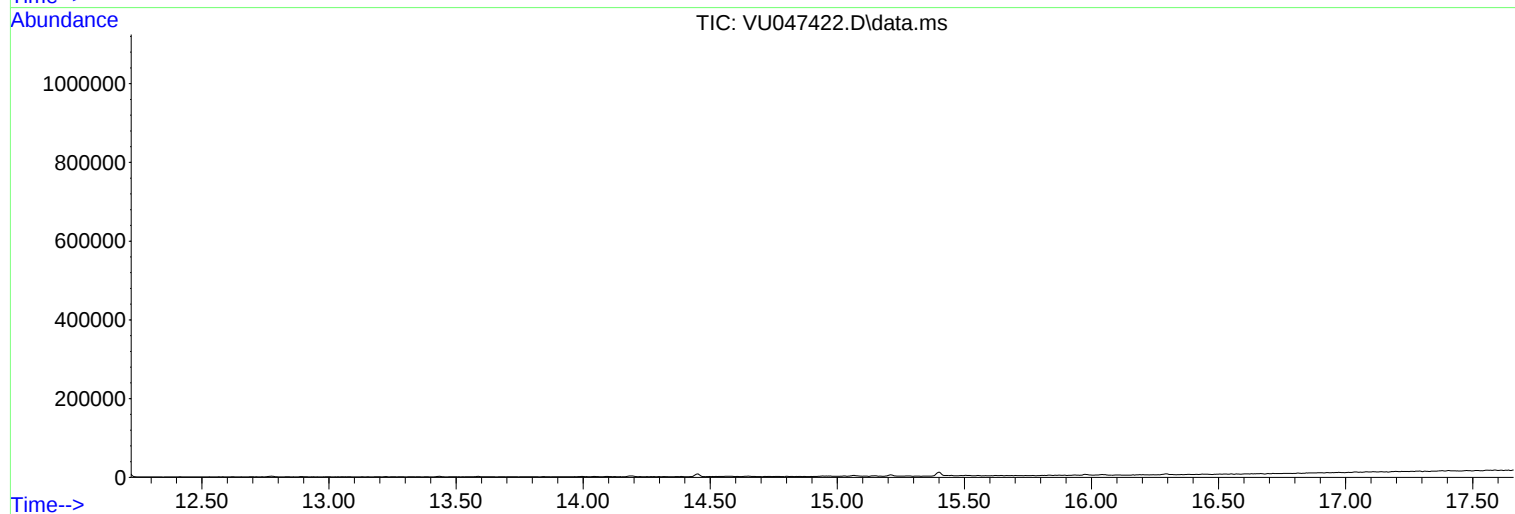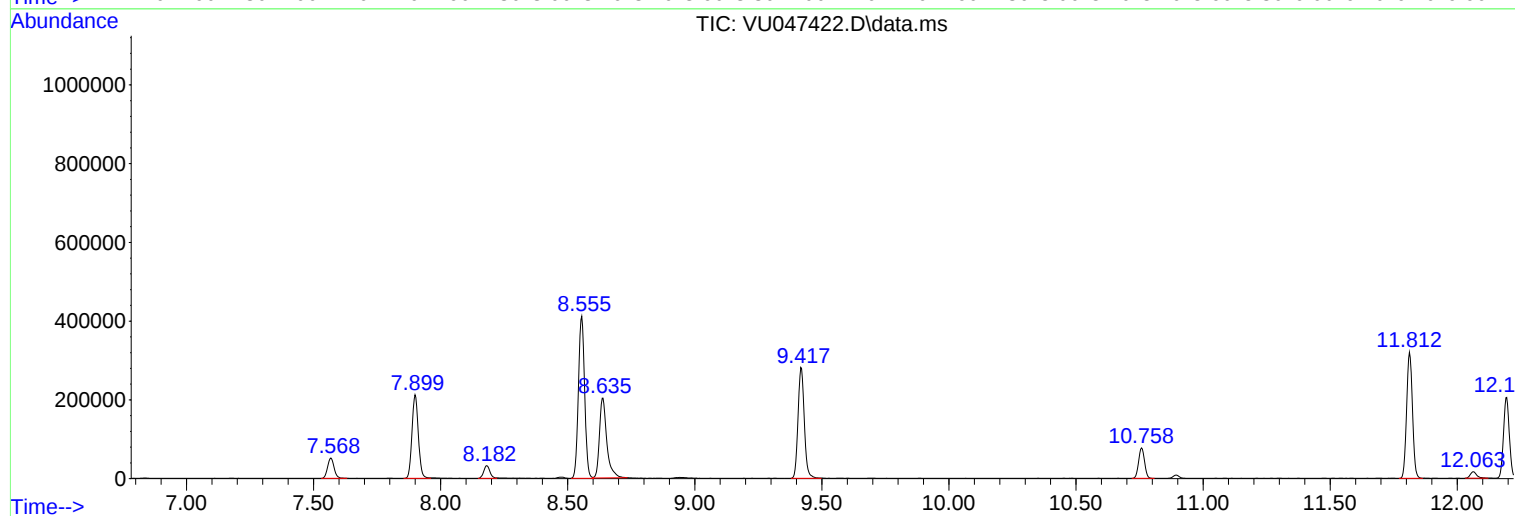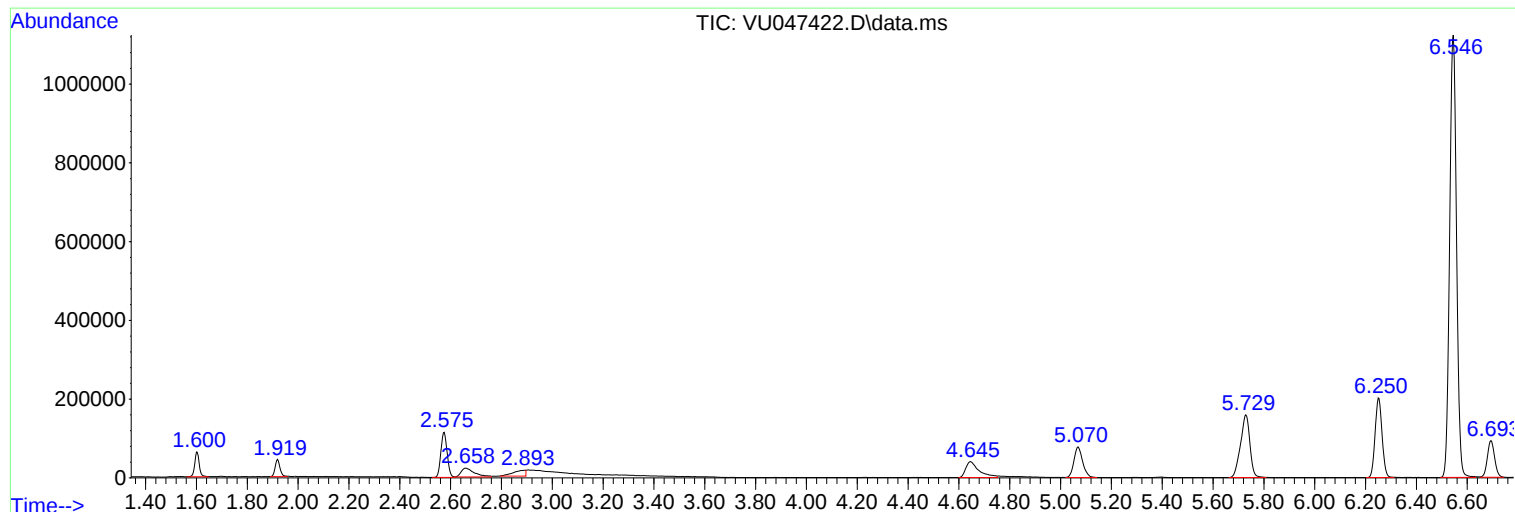

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030922\
Data File : VU047422.D
Acq On : 09 Mar 2022 22:17
Operator : SY/MD
Sample : N1861-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YATM0










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.893	0.67 ug/L	51578	1,4-Difluorobenzene	6.250

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
4			4-Penten-2-ol	86	C5H10O	000625-31-0	9
5			Formamide	45	CH3NO	000075-12-7	7

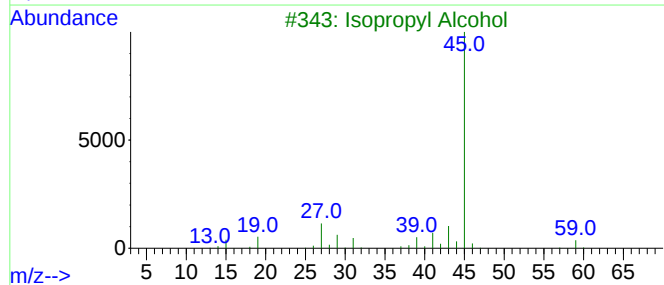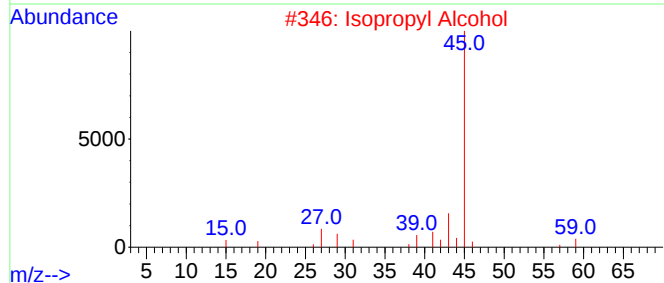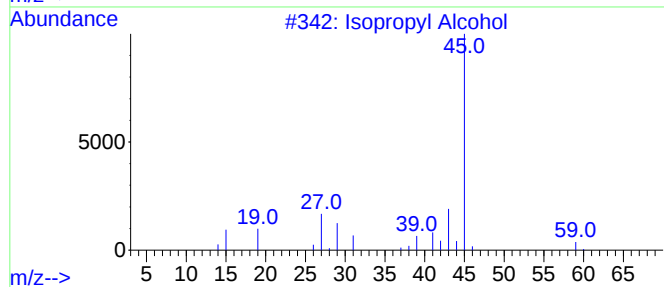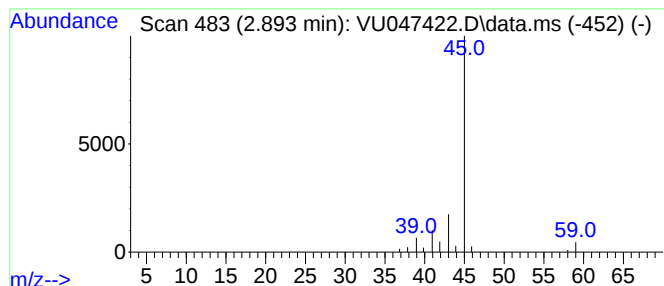

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030922\
Data File : VU047422.D
Acq On : 09 Mar 2022 22:17
Operator : SY/MD
Sample : N1861-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YATM0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.893	0.7	ug/L	51578	1	6.250	384833	5.0