

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030922\
 Data File : VU047426.D
 Acq On : 09 Mar 2022 23:51
 Operator : SY/MD
 Sample : N1861-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YBIB3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU047426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.491	41	47	52	rBV3	4660	5283	1.07%	0.129%
2	1.604	72	82	99	rVB2	83140	98206	19.86%	2.399%
3	1.919	171	180	198	rBV	43257	58741	11.88%	1.435%
4	2.575	370	384	397	rBV	107685	175277	35.45%	4.282%
5	2.655	397	409	437	rVV	9055	30405	6.15%	0.743%
6	4.642	1012	1027	1060	rBV	37758	134688	27.24%	3.290%
7	5.070	1143	1160	1179	rVB	74919	174167	35.23%	4.255%
8	5.391	1245	1260	1273	rBV2	8929	20216	4.09%	0.494%
9	5.729	1345	1365	1391	rBV2	158266	401283	81.17%	9.803%
10	6.250	1514	1527	1555	rBV	197348	375006	75.85%	9.161%
11	6.539	1608	1617	1627	rVB8	2978	5665	1.15%	0.138%
12	6.694	1652	1665	1683	rBV	90319	177745	35.95%	4.342%
13	7.169	1803	1813	1826	rVB3	3161	5772	1.17%	0.141%
14	7.568	1925	1937	1951	rBV	50713	88559	17.91%	2.163%
15	7.899	2027	2040	2056	rBV	208144	358936	72.60%	8.769%
16	8.182	2114	2128	2143	rBV	30369	53023	10.73%	1.295%
17	8.485	2209	2222	2235	rBV4	5123	10624	2.15%	0.260%
18	8.555	2235	2244	2254	rVB3	12114	18791	3.80%	0.459%
19	8.639	2254	2270	2312	rBV	200503	426326	86.24%	10.415%
20	9.417	2498	2512	2533	rBV	273232	465570	94.17%	11.373%
21	10.758	2917	2929	2948	rVB	73097	120431	24.36%	2.942%
22	10.893	2960	2971	2982	rBV2	6784	11061	2.24%	0.270%
23	11.812	3244	3257	3277	rBV	315426	494375	100.00%	12.077%
24	12.063	3324	3335	3351	rBV2	25809	44400	8.98%	1.085%
25	12.192	3364	3375	3395	rVB	200909	325786	65.90%	7.959%
26	14.449	4069	4077	4085	rVB4	4527	5935	1.20%	0.145%
27	15.401	4365	4373	4383	rBV6	5327	7198	1.46%	0.176%




Sum of corrected areas: 4093469

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030922\
Data File : VU047426.D
Acq On : 09 Mar 2022 23:51
Operator : SY/MD
Sample : N1861-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YBIB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

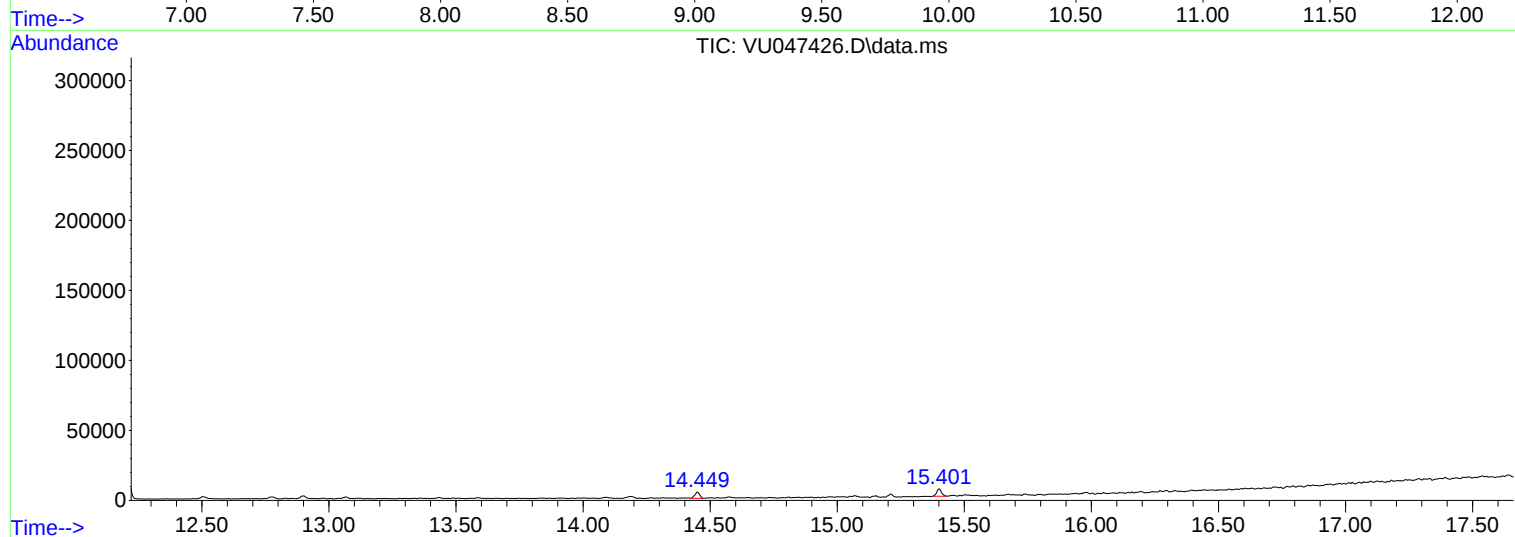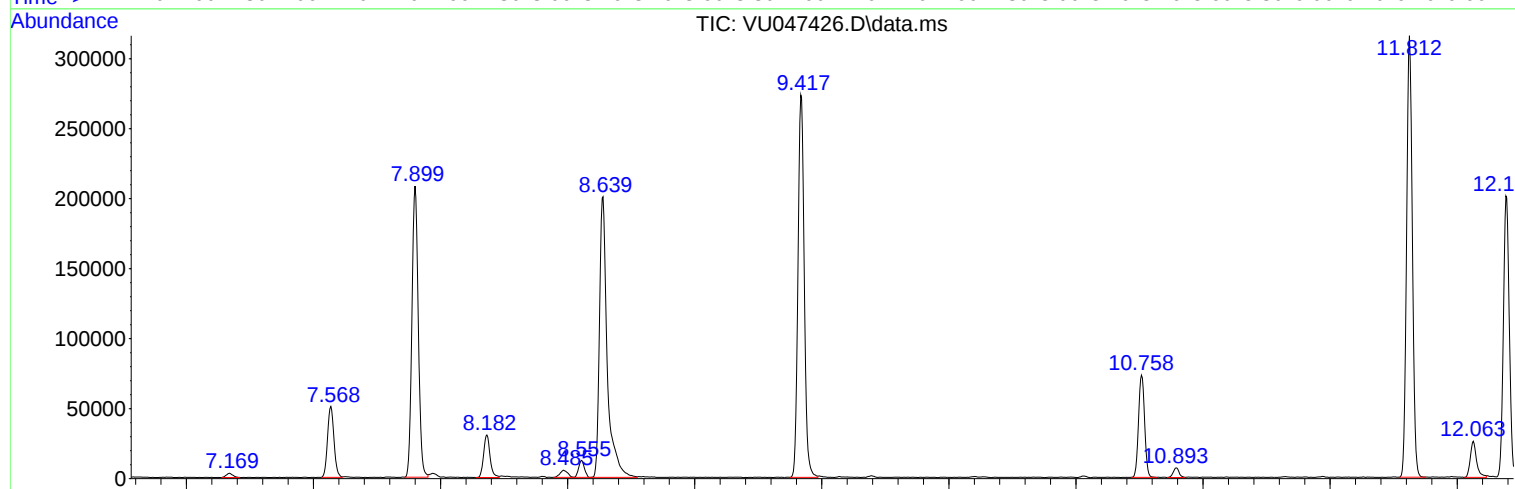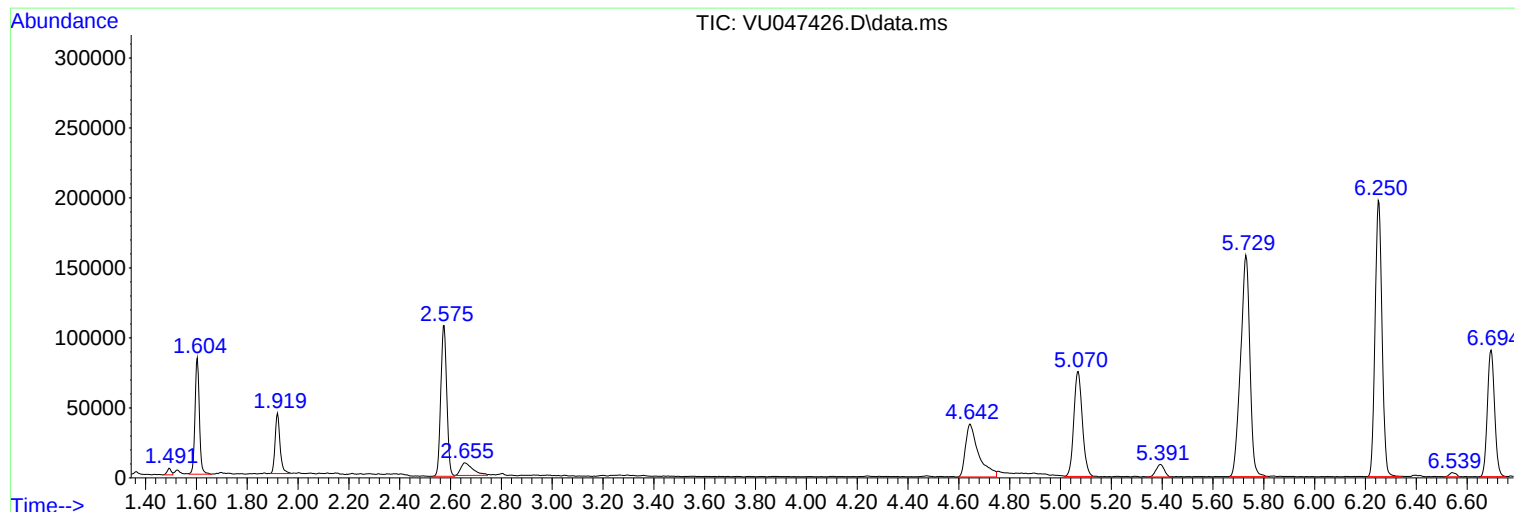

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030922\
Data File : VU047426.D
Acq On : 09 Mar 2022 23:51
Operator : SY/MD
Sample : N1861-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YBIB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030922\
Data File : VU047426.D
Acq On : 09 Mar 2022 23:51
Operator : SY/MD
Sample : N1861-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YBIB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------