


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030922\
 Data File : VU047399.D
 Acq On : 09 Mar 2022 09:04
 Operator : SY/MD
 Sample : BFB064
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB064

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Mar 14 12:06:39 2022

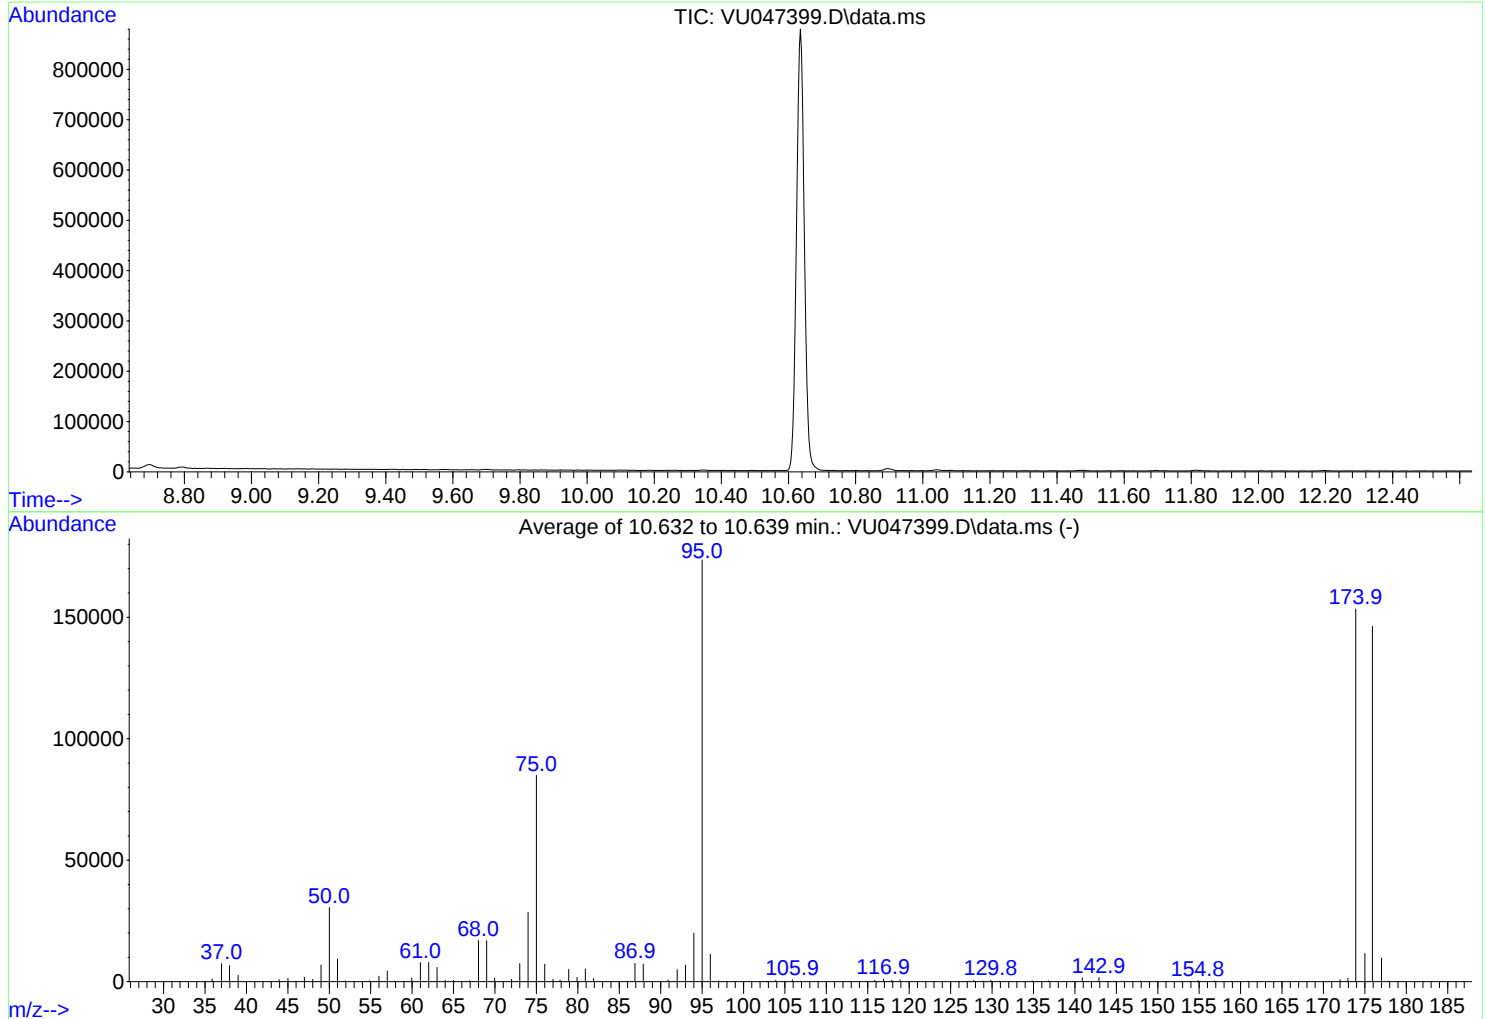

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	30547	PASS
75	95	30	80	48.9	84907	PASS
95	95	100	100	100.0	173653	PASS
96	95	5	9	6.5	11266	PASS
173	174	0.00	2	0.9	1369	PASS
174	95	50	120	88.3	153365	PASS
175	174	5	9	7.6	11589	PASS
176	174	95	101	95.4	146283	PASS
177	176	5	9	6.6	9658	PASS

m/z	Abundance
35.90	1246.0
37.90	496.0
39.90	554.0
43.90	333.0
207.00	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

m/z	Abundance
35.90	2471.0
37.00	7354.0
38.00	7091.0
39.00	2615.0
39.90	581.0
42.80	109.0
44.00	1140.0
45.00	1282.0
46.00	180.0
47.00	1843.0
48.00	928.0
49.00	6798.0
50.00	30928.0
51.00	9427.0
51.90	376.0
54.90	433.0
56.00	2305.0
57.00	4557.0
57.90	206.0
59.90	1502.0
61.00	7909.0
62.00	8006.0
63.00	5905.0
64.00	516.0
65.00	524.0
67.00	380.0
68.00	17288.0
69.00	17184.0
69.90	1388.0
72.00	916.0
73.00	7717.0
74.00	28800.0
75.00	85104.0
76.00	7364.0
77.00	958.0
77.90	652.0
78.90	5114.0
79.90	1706.0
80.90	5116.0
81.90	1299.0
82.90	144.0
85.90	160.0
86.90	7617.0
87.90	7264.0
90.90	637.0
92.00	4957.0
93.00	6977.0
94.00	19744.0
95.00	173056.0
96.00	11506.0
97.00	302.0
103.90	597.0
104.90	243.0
105.90	724.0
106.90	206.0
110.80	131.0
112.80	157.0
114.80	191.0
115.80	583.0
116.90	1090.0
117.90	698.0
118.90	767.0
125.90	116.0
127.80	578.0
128.90	252.0
129.90	628.0
130.90	174.0
134.90	329.0
136.80	271.0
139.80	121.0
140.90	1551.0
141.90	181.0
142.90	1788.0
144.80	197.0
145.90	252.0
146.80	100.0
147.90	326.0
148.90	106.0
149.70	167.0
151.80	108.0
152.90	192.0
154.80	444.0
156.90	271.0
158.90	193.0
160.90	205.0
172.00	832.0
173.00	1432.0
173.90	148544.0
175.00	11304.0
175.90	142336.0
177.00	9721.0
177.90	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

m/z	Abundance
35.00	2477.0
37.00	7535.0
38.00	7242.0
39.00	2641.0
39.00	575.0
44.00	1171.0
45.00	1339.0
46.00	168.0
47.00	1886.0
48.00	960.0
49.00	7126.0
50.00	31520.0
51.00	9596.0
51.00	377.0
54.00	427.0
56.00	2323.0
57.00	4575.0
57.00	209.0
59.00	1513.0
61.00	8149.0
62.00	8175.0
63.00	6064.0
64.00	516.0
65.00	538.0
67.00	370.0
68.00	17400.0
69.00	17400.0
70.00	1457.0
72.00	930.0
73.00	7649.0
74.00	29312.0
75.00	87656.0
76.00	7384.0
77.00	1051.0
77.00	680.0
78.00	5135.0
79.00	1814.0
80.00	5375.0
81.00	1289.0
82.00	146.0
85.00	185.0
86.00	7749.0
87.00	7528.0
90.00	693.0
92.00	5106.0
93.00	6995.0
94.00	20552.0
95.00	179200.0
96.00	11579.0
97.00	331.0
102.80	115.0
103.90	619.0
104.90	219.0
105.90	742.0
106.90	227.0
110.80	136.0
112.80	163.0
114.80	192.0
115.80	583.0
116.90	1129.0
117.90	622.0
118.90	764.0
127.80	603.0
128.90	293.0
129.80	604.0
130.90	198.0
134.80	319.0
136.80	326.0
139.80	131.0
140.90	1580.0
142.00	209.0
142.90	1795.0
143.80	117.0
144.80	175.0
145.90	305.0
146.80	134.0
147.90	331.0
148.80	123.0
149.70	197.0
151.80	103.0
152.90	187.0
153.80	108.0
154.80	472.0
156.90	298.0
159.00	206.0
160.90	256.0
172.00	829.0
172.90	1420.0
173.90	158336.0
175.00	12041.0
175.90	150528.0
177.00	9988.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

177.90

258.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

m/z	Abundance
35.00	2338.0
37.00	7174.0
38.00	6857.0
39.00	2431.0
39.00	595.0
44.00	1110.0
45.00	1321.0
46.00	121.0
47.00	1687.0
48.00	899.0
49.00	6660.0
50.00	29192.0
51.00	8951.0
52.00	344.0
54.00	383.0
56.00	2155.0
57.00	4213.0
57.00	195.0
60.00	1396.0
61.00	7506.0
62.00	7594.0
63.00	5529.0
64.00	493.0
65.00	528.0
66.00	376.0
68.00	15860.0
69.00	16115.0
70.00	1341.0
72.00	846.0
73.00	7045.0
74.00	27416.0
75.00	81960.0
76.00	6859.0
77.00	1012.0
77.00	670.0
78.00	4767.0
79.00	1748.0
80.00	5062.0
81.00	1151.0
83.00	126.0
86.00	189.0
86.00	7288.0
87.00	7055.0
90.00	643.0
92.00	4765.0
93.00	6562.0
94.00	19576.0
95.00	168704.0
96.00	10712.0
97.00	314.0
103.00	616.0
105.00	182.0
105.00	650.0
106.00	207.0
110.00	117.0
112.00	157.0
114.00	187.0
115.00	521.0
116.00	1037.0
117.00	517.0
118.00	739.0
127.00	542.0
128.00	293.0
129.00	571.0
130.00	229.0
134.00	281.0
136.00	334.0
139.00	123.0
140.00	1490.0
141.00	198.0
142.00	1669.0
143.00	108.0
144.00	162.0
146.00	298.0
146.00	134.0
147.00	337.0
148.00	139.0
149.00	199.0
152.00	158.0
153.00	124.0
154.00	429.0
156.00	288.0
159.00	191.0
160.00	238.0
172.00	790.0
173.00	1254.0
173.00	153216.0
175.00	11423.0
175.00	145984.0
177.00	9266.0
177.00	261.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064