

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031022\
 Data File : VU047466.D
 Acq On : 10 Mar 2022 18:25
 Operator : SY/MD
 Sample : VIBLK012
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK012

Quant Time: Mar 11 00:57:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 11 00:52:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	135681	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	129812	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	66041	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	35915	4.881	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.600%
7) Chloroethane-d5	1.919	69	27498	5.090	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.800%
11) 1,1-Dichloroethene-d2	2.572	65	16421	5.052	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	101.000%
20) 2-Butanone-d5	4.646	46	69289	52.886	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.780%
24) Chloroform-d	5.067	84	59516	5.077	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.600%
26) 1,2-Dichloroethane-d4	5.707	65	30798	5.188	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.800%
32) Benzene-d6	5.729	84	126399	5.176	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.600%
36) 1,2-Dichloropropane-d6	6.694	67	38096	5.274	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.400%
41) Toluene-d8	7.899	98	116707	4.863	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.200%
43) trans-1,3-Dichloroprop...	8.182	79	14852	4.843	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.800%
46) 2-Hexanone-d5	8.639	63	66375	49.129	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.260%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	31321	4.975	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.600%
66) 1,2-Dichlorobenzene-d4	12.195	152	45597	5.446	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.000%
Target Compounds						Qvalue
22) cis-1,2-Dichloroethene	4.668	96	485	0.051	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031022\
Data File : VU047466.D
Acq On : 10 Mar 2022 18:25
Operator : SY/MD
Sample : VIBLK012
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK012


Quant Time: Mar 11 00:57:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 11 00:52:41 2022
Response via : Initial Calibration

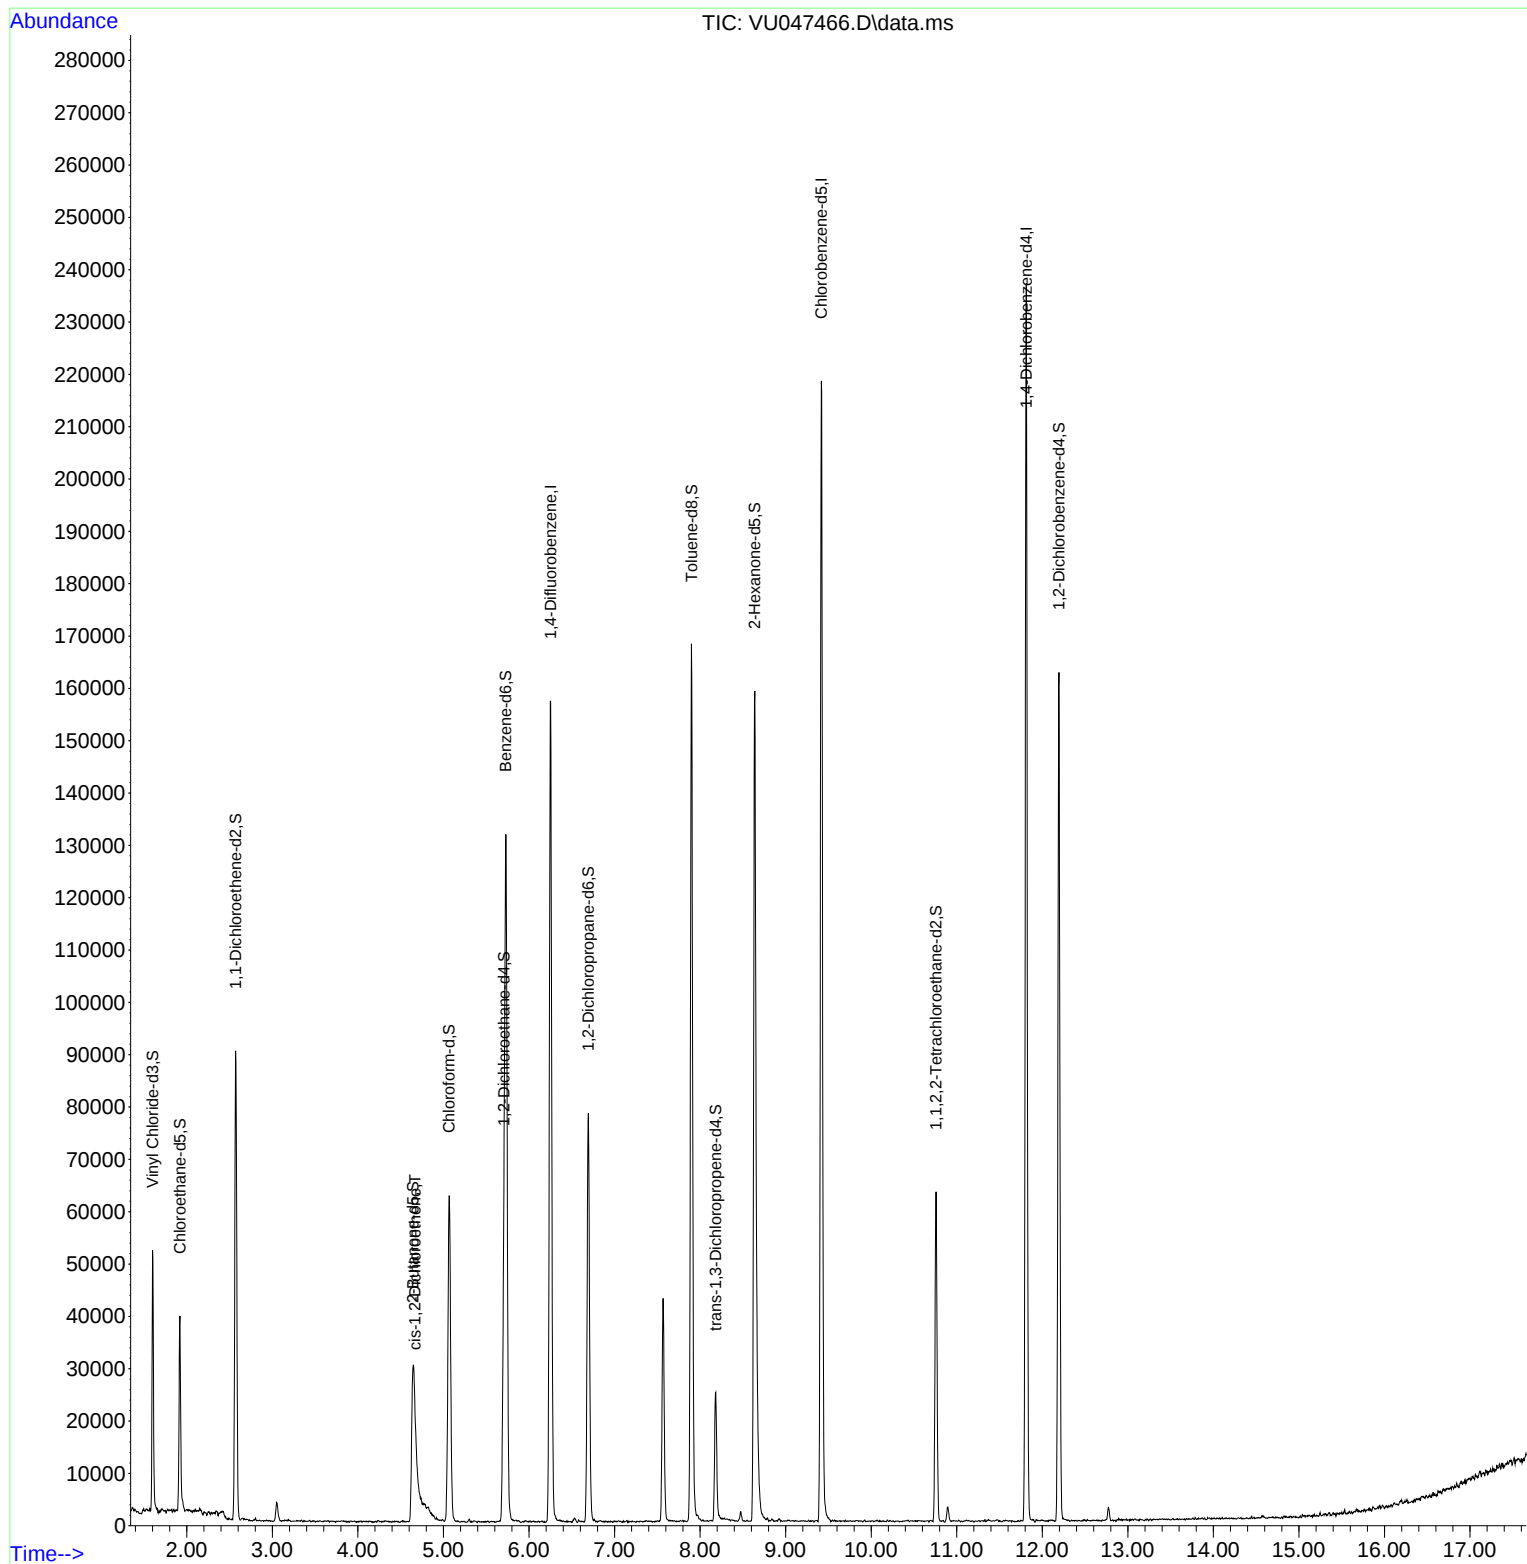

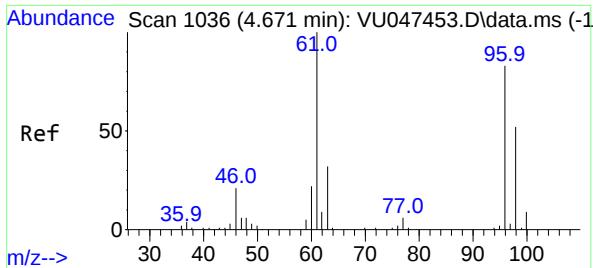

cis-1,2-Dichloroethene
 Concen: 0.051 ug/L
 RT: 4.668 min Scan# 10
 Delta R.T. -0.003 min
 Lab File: VU047466.D
 Acq: 10 Mar 2022 18:25

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK012

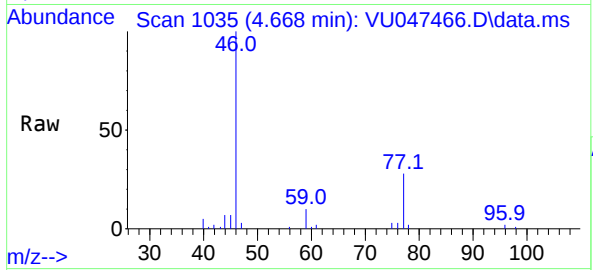

Tgt Ion: 96 Resp: 485

Ion	Ratio	Lower	Upper
96	100		
61	93.6	80.8	150.0
98	58.8	44.7	83.1

