

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031022\
 Data File : VU047458.D
 Acq On : 10 Mar 2022 15:16
 Operator : SY/MD
 Sample : N1810-23
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU047458.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	92	rBV	55334	61974	14.32%	1.736%
2	1.919	172	180	199	rVB	40038	54352	12.56%	1.523%
3	2.572	372	383	400	rVB	97631	158682	36.67%	4.446%
4	2.890	459	482	483	rBV4	2591	7317	1.69%	0.205%
5	3.051	527	532	544	rVB4	4595	7498	1.73%	0.210%
6	3.189	564	575	591	rVB	5710	13199	3.05%	0.370%
7	4.646	1008	1028	1065	rBV2	41473	167638	38.74%	4.697%
8	5.070	1143	1160	1179	rBV	69348	153596	35.50%	4.303%
9	5.729	1343	1365	1391	rBV2	144463	366533	84.71%	10.270%
10	6.250	1512	1527	1545	rBV	172984	328109	75.83%	9.193%
11	6.694	1650	1665	1683	rBV	86082	166725	38.53%	4.671%
12	7.568	1924	1937	1958	rBV	45704	81291	18.79%	2.278%
13	7.899	2025	2040	2062	rBV	186643	324646	75.03%	9.096%
14	8.182	2117	2128	2143	rBV	28394	49183	11.37%	1.378%
15	8.475	2211	2219	2229	rVB4	3103	5406	1.25%	0.151%
16	8.639	2257	2270	2297	rBV	178183	360583	83.34%	10.103%
17	9.417	2499	2512	2541	rBV	241862	409069	94.54%	11.461%
18	10.758	2918	2929	2944	rVB	70112	112033	25.89%	3.139%
19	10.896	2959	2972	2982	rVB2	9093	14656	3.39%	0.411%
20	11.812	3244	3257	3275	rBV	273944	432678	100.00%	12.123%
21	12.192	3364	3375	3390	rBV	181879	293944	67.94%	8.236%




Sum of corrected areas: 3569112

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031022\
Data File : VU047458.D
Acq On : 10 Mar 2022 15:16
Operator : SY/MD
Sample : N1810-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

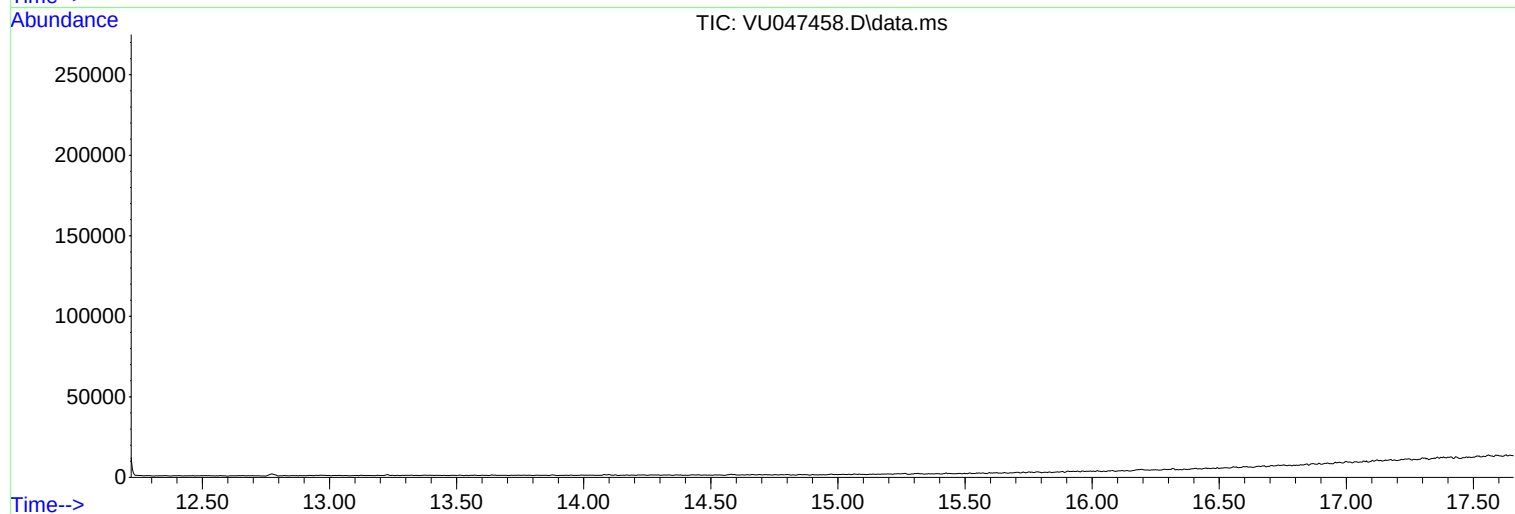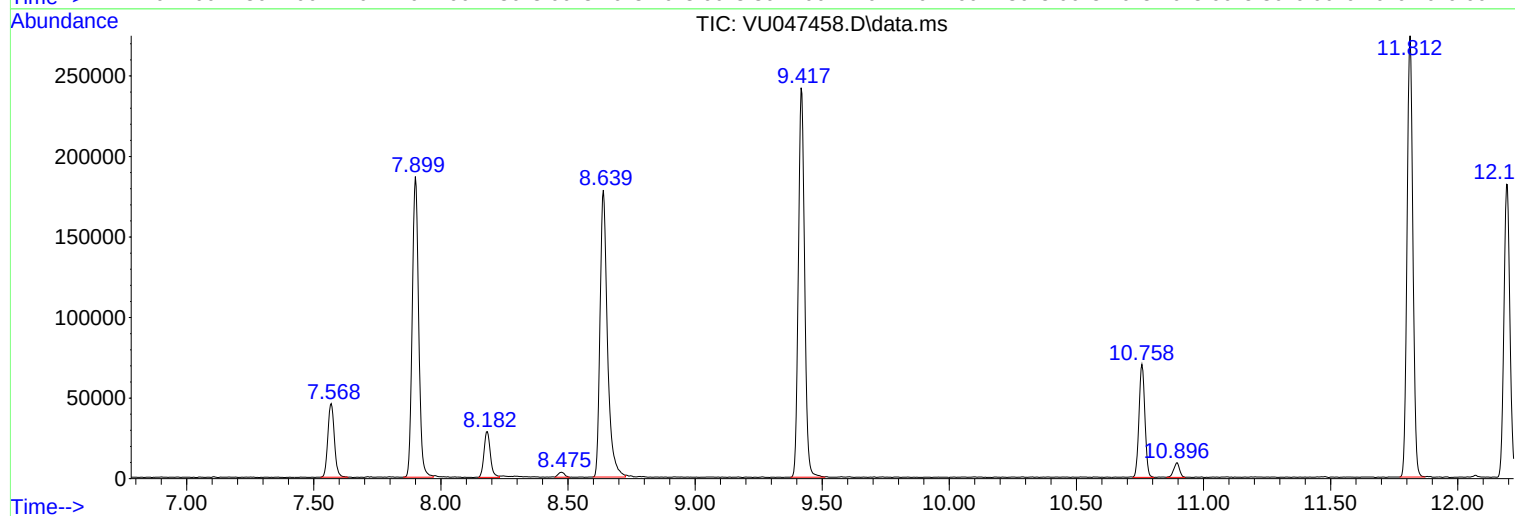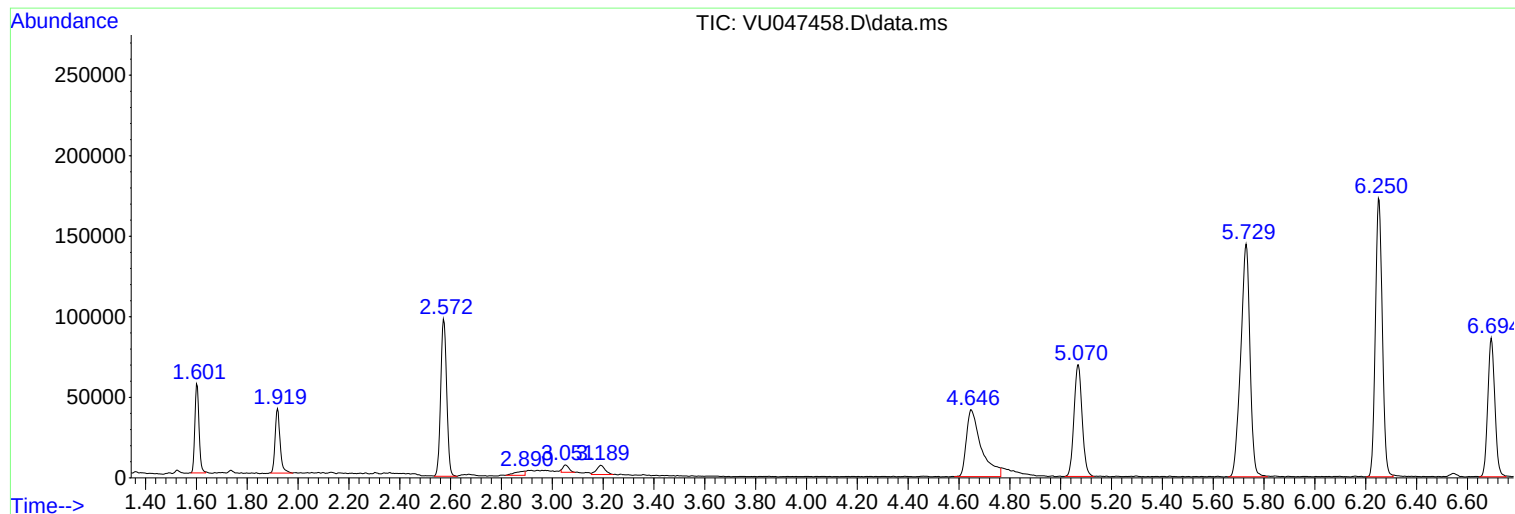

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031022\
Data File : VU047458.D
Acq On : 10 Mar 2022 15:16
Operator : SY/MD
Sample : N1810-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031022\
Data File : VU047458.D
Acq On : 10 Mar 2022 15:16
Operator : SY/MD
Sample : N1810-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------