
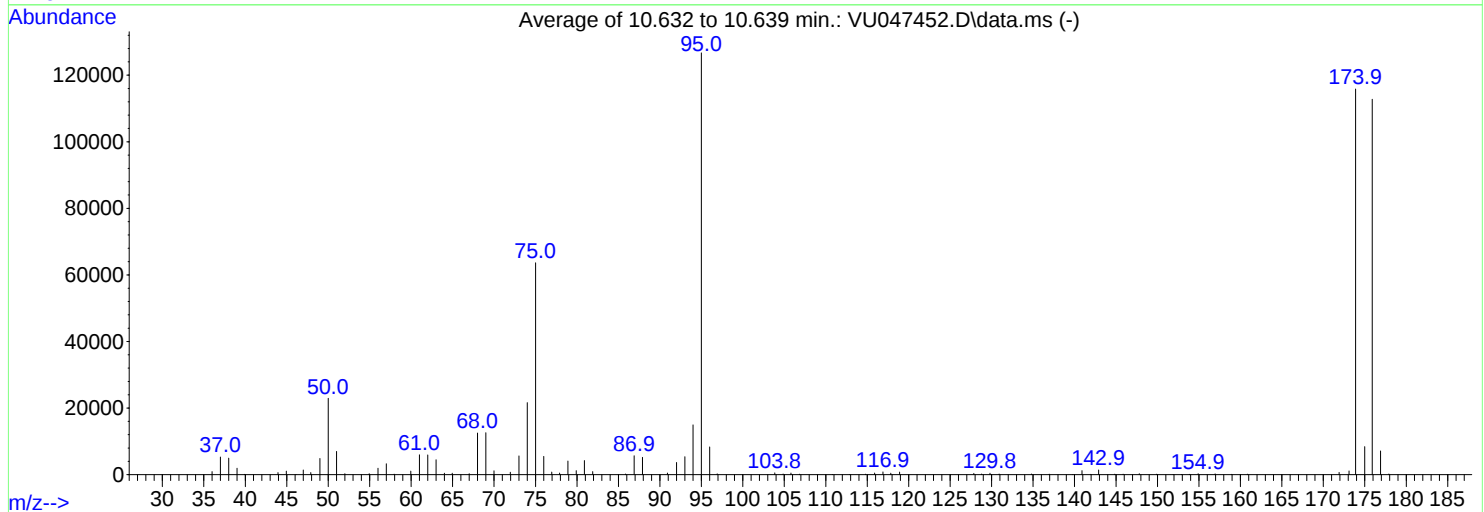


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031022\
 Data File : VU047452.D
 Acq On : 10 Mar 2022 11:43
 Operator : SY/MD
 Sample : BFB065
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB065

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Mar 14 12:06:39 2022

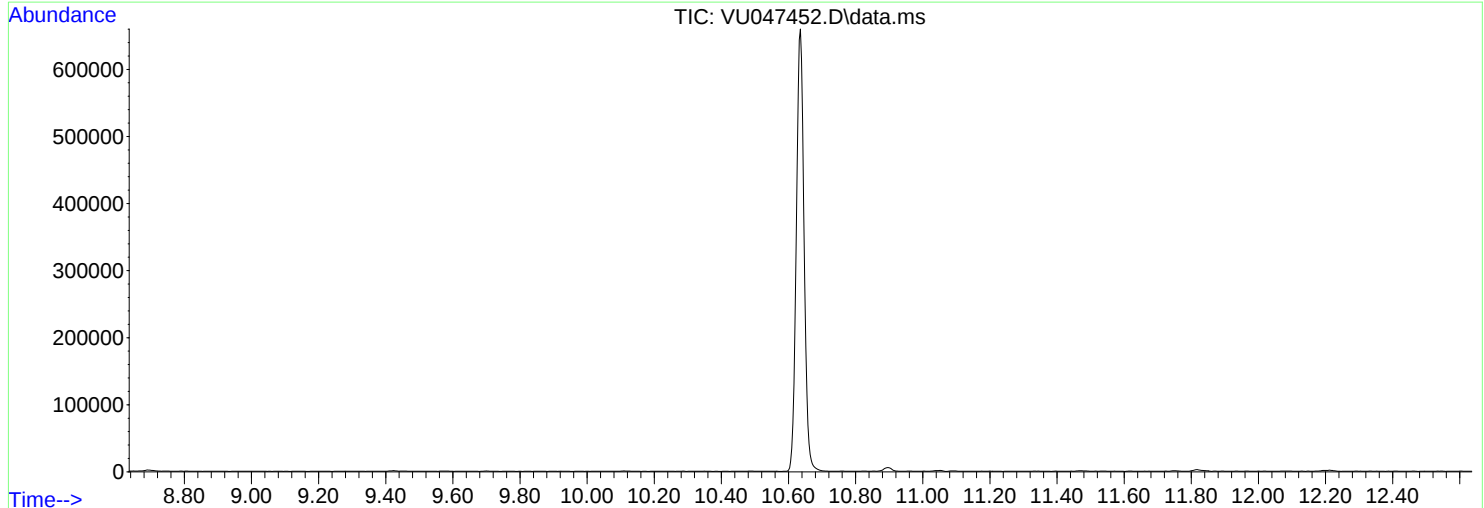

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	22912	PASS
75	95	30	80	50.2	63637	PASS
95	95	100	100	100.0	126717	PASS
96	95	5	9	6.6	8336	PASS
173	174	0.00	2	0.9	1095	PASS
174	95	50	120	91.4	115851	PASS
175	174	5	9	7.3	8432	PASS
176	174	95	101	97.3	112755	PASS
177	176	5	9	6.3	7127	PASS

Scan 2876 (10.587 min): VU047452.D\data.ms
BFB065

m/z	Abundance
39.90	511.0
44.00	263.0
206.80	141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065

m/z	Abundance
36.00	982.0
37.00	5416.0
38.00	5123.0
39.00	1981.0
39.90	619.0
44.00	885.0
45.00	1060.0
46.10	114.0
47.00	1417.0
47.90	702.0
49.00	4896.0
50.00	23448.0
51.00	7275.0
52.00	351.0
55.00	313.0
56.00	2042.0
57.00	3393.0
57.90	170.0
60.00	1119.0
61.00	6172.0
62.00	5874.0
63.00	4478.0
64.00	476.0
64.90	438.0
67.00	280.0
68.00	12641.0
69.00	12929.0
70.00	1144.0
72.00	765.0
73.00	5814.0
74.00	22008.0
75.00	64768.0
76.00	5690.0
77.00	835.0
77.90	508.0
78.90	4151.0
79.90	1186.0
80.90	4236.0
81.90	961.0
85.80	200.0
86.90	5678.0
87.90	5283.0
90.90	445.0
92.00	3640.0
93.00	5561.0
94.00	15143.0
95.00	128736.0
96.00	8581.0
96.90	248.0
103.90	599.0
104.80	211.0
105.80	500.0
106.90	130.0
114.80	152.0
115.90	501.0
116.90	866.0
117.90	466.0
118.90	760.0
127.80	436.0
128.80	211.0
129.80	407.0
130.90	200.0
134.80	222.0
136.90	149.0
140.90	1254.0
142.00	127.0
142.90	1333.0
144.90	173.0
145.80	180.0
147.80	270.0
149.90	159.0
152.90	103.0
153.80	124.0
154.90	257.0
156.90	224.0
159.00	127.0
160.90	129.0
171.90	696.0
173.10	1151.0
173.90	114408.0
175.00	8538.0
175.90	111232.0
176.90	7066.0
177.90	189.0
207.00	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065

m/z	Abundance
36.00	973.0
37.00	5426.0
38.00	5162.0
39.00	1950.0
39.90	628.0
44.00	935.0
44.90	1092.0
47.00	1432.0
47.90	655.0
49.00	5003.0
50.00	23656.0
51.00	7188.0
52.00	330.0
54.90	313.0
56.00	2029.0
57.00	3392.0
58.00	153.0
59.90	1097.0
61.00	6179.0
62.00	6121.0
63.00	4611.0
64.00	481.0
65.00	441.0
67.00	282.0
68.00	12949.0
69.00	12946.0
70.00	1239.0
72.00	730.0
73.00	5841.0
74.00	22376.0
75.00	65736.0
76.00	5687.0
76.90	793.0
77.90	516.0
78.90	4203.0
79.90	1237.0
80.90	4393.0
81.90	989.0
85.80	185.0
86.90	5846.0
87.90	5423.0
90.90	479.0
92.00	3826.0
93.00	5552.0
94.00	15384.0
95.00	130712.0
96.00	8522.0
96.90	271.0
103.80	585.0
104.90	190.0
105.80	530.0
106.90	150.0
110.80	113.0
114.80	140.0
115.90	504.0
116.90	859.0
117.80	484.0
118.90	791.0
127.80	419.0
128.80	227.0
129.80	442.0
130.90	197.0
134.80	214.0
137.00	172.0
139.80	101.0
140.90	1231.0
141.90	136.0
142.90	1427.0
144.90	173.0
145.80	167.0
147.80	281.0
149.90	173.0
151.90	102.0
152.90	112.0
153.90	120.0
154.90	305.0
156.90	255.0
159.00	122.0
160.80	142.0
171.90	724.0
173.10	1140.0
173.90	119544.0
175.00	8738.0
175.90	116152.0
176.90	7344.0
177.90	192.0
207.00	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065

m/z	Abundance
36.00	871.0
37.00	4993.0
38.00	4567.0
39.00	1810.0
39.90	659.0
43.90	904.0
44.90	1008.0
47.00	1332.0
47.90	568.0
49.00	4659.0
50.00	21632.0
51.00	6484.0
52.00	271.0
54.90	283.0
56.00	1758.0
57.00	3010.0
58.00	123.0
60.00	977.0
61.00	5622.0
62.00	5719.0
63.00	4318.0
64.00	422.0
65.00	433.0
67.00	280.0
68.00	11976.0
69.00	11874.0
70.00	1157.0
71.90	648.0
73.00	5287.0
74.00	20464.0
75.00	60408.0
76.00	5093.0
76.90	731.0
77.90	449.0
78.90	3880.0
79.90	1199.0
80.90	4052.0
81.90	877.0
85.90	152.0
86.90	5448.0
87.90	4902.0
90.90	489.0
92.00	3473.0
93.00	5040.0
94.00	14345.0
95.00	120704.0
96.00	7904.0
96.90	247.0
103.90	488.0
104.90	151.0
105.80	501.0
106.80	142.0
112.90	106.0
114.80	121.0
115.90	489.0
116.90	794.0
117.80	423.0
118.90	738.0
127.90	390.0
128.80	224.0
129.80	417.0
130.90	178.0
134.80	194.0
137.00	188.0
139.80	105.0
140.90	1113.0
141.90	119.0
142.90	1386.0
144.80	156.0
145.90	147.0
147.80	275.0
149.90	141.0
154.90	310.0
157.00	230.0
158.90	108.0
160.80	124.0
171.90	674.0
173.10	993.0
173.90	113600.0
175.00	8020.0
175.90	110880.0
176.90	6970.0
177.90	171.0
207.00	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065