

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
 Data File : VU047510.D
 Acq On : 11 Mar 2022 22:42
 Operator : SY/MD
 Sample : N1909-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YATN9

Quant Time: Mar 12 04:23:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 12 03:24:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	123852	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	120134	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	63097	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	28417	4.231	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.600%
7) Chloroethane-d5	1.919	69	22587	4.580	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.600%
11) 1,1-Dichloroethene-d2	2.571	65	13032	4.392	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.800%
20) 2-Butanone-d5	4.649	46	59172	49.478	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.960%
24) Chloroform-d	5.070	84	50673	4.735	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
26) 1,2-Dichloroethane-d4	5.706	65	26628	4.914	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.200%
32) Benzene-d6	5.729	84	101927	4.511	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.200%
36) 1,2-Dichloropropane-d6	6.694	67	31347	4.689	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.800%
41) Toluene-d8	7.899	98	93607	4.214	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.200%
43) trans-1,3-Dichloroprop...	8.182	79	12085	4.258	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.200%
46) 2-Hexanone-d5	8.639	63	56685	45.337	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.680%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	28488	4.890	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.800%
66) 1,2-Dichlorobenzene-d4	12.195	152	38791	4.849	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.000%
Target Compounds						
					Qvalue	
13) Acetone	2.662	43	65898	59.973	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
Data File : VU047510.D
Acq On : 11 Mar 2022 22:42
Operator : SY/MD
Sample : N1909-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YATN9

Quant Time: Mar 12 04:23:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Mar 12 03:24:52 2022
Response via : Initial Calibration

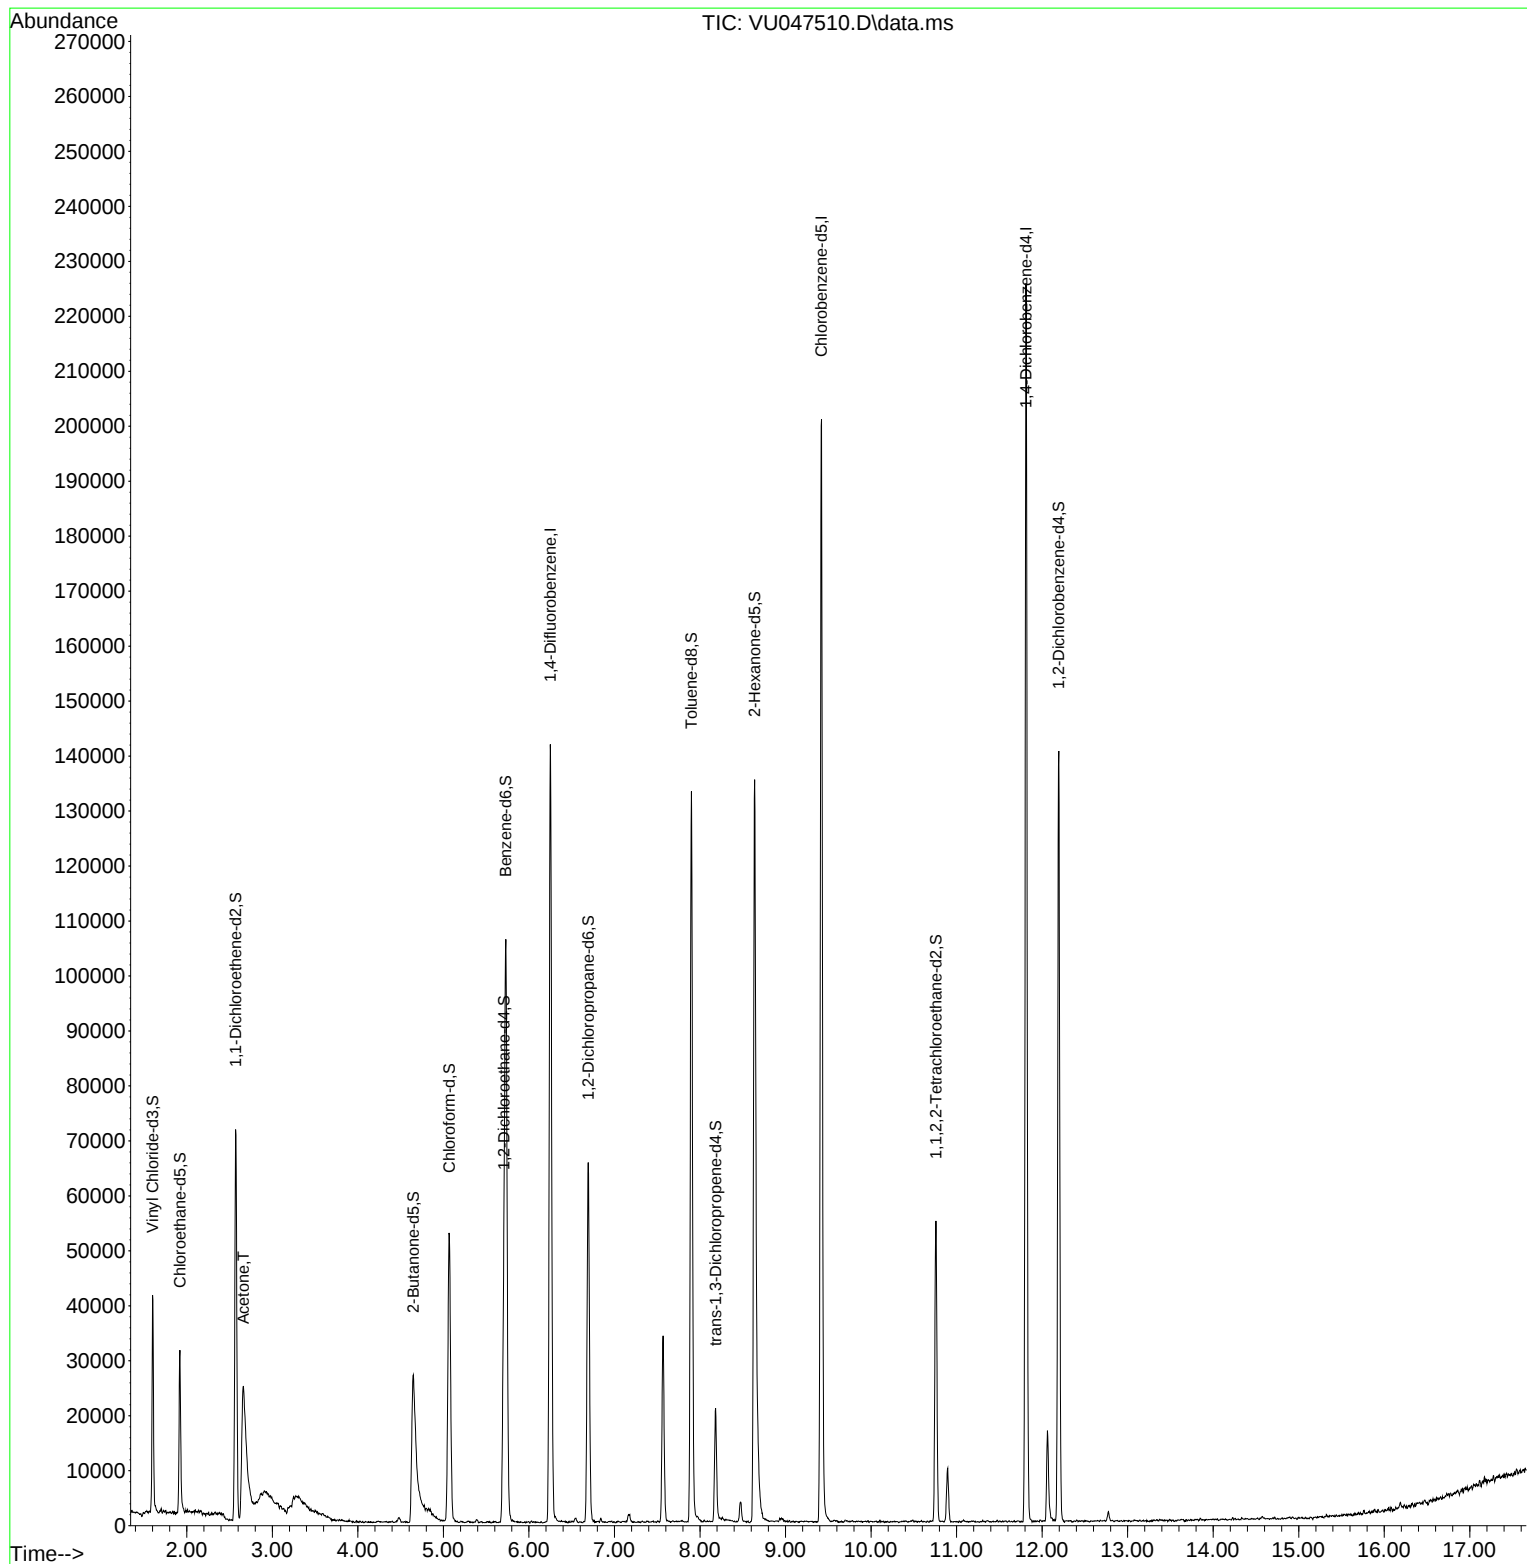

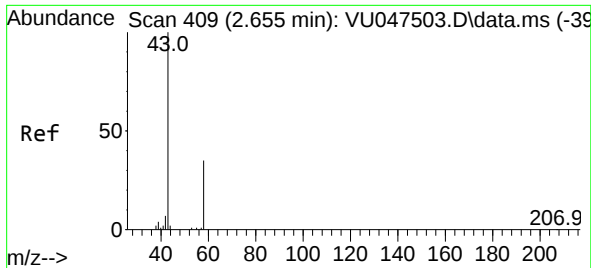

#13

Acetone

Concen: 59.973 ug/L

RT: 2.662 min Scan# 411

Delta R.T. 0.007 min

Lab File: VU047510.D


Acq: 11 Mar 2022 22:42

Instrument :

MSVOA_U

ClientSampleId :

YATN9

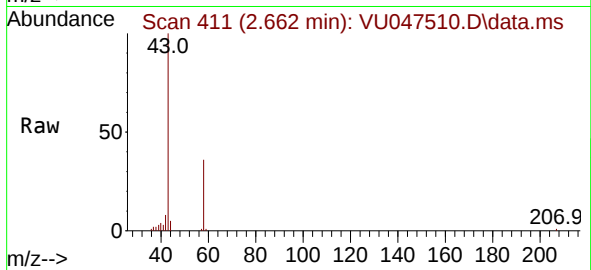

Tgt Ion: 43 Resp: 65898

Ion Ratio Lower Upper

43 100

58 33.5 0.0 72.6

