

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
 Data File : VU047523.D
 Acq On : 12 Mar 2022 03:48
 Operator : SY/MD
 Sample : N1858-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNK6

Quant Time: Mar 14 01:44:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Mar 12 03:24:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	113196	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	111920	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	56895	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	25397	4.137	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.800%
7) Chloroethane-d5	1.919	69	20659	4.584	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.600%
11) 1,1-Dichloroethene-d2	2.571	65	11783	4.345	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.000%
20) 2-Butanone-d5	4.649	46	55420	50.703	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.400%
24) Chloroform-d	5.067	84	47695	4.877	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%
26) 1,2-Dichloroethane-d4	5.706	65	24357	4.918	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.400%
32) Benzene-d6	5.732	84	96346	4.576	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
36) 1,2-Dichloropropane-d6	6.693	67	29449	4.728	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.600%
41) Toluene-d8	7.899	98	84964	4.106	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.200%
43) trans-1,3-Dichloroprop...	8.182	79	10857	4.106	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.200%
46) 2-Hexanone-d5	8.639	63	50105	43.015	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.020%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	26267	4.840	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.800%
66) 1,2-Dichlorobenzene-d4	12.195	152	36019	4.993	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.800%
Target Compounds						
					Qvalue	
3) Chloromethane	1.523	50	1382	0.163	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
Data File : VU047523.D
Acq On : 12 Mar 2022 03:48
Operator : SY/MD
Sample : N1858-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNK6


Quant Time: Mar 14 01:44:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Mar 12 03:24:52 2022
Response via : Initial Calibration

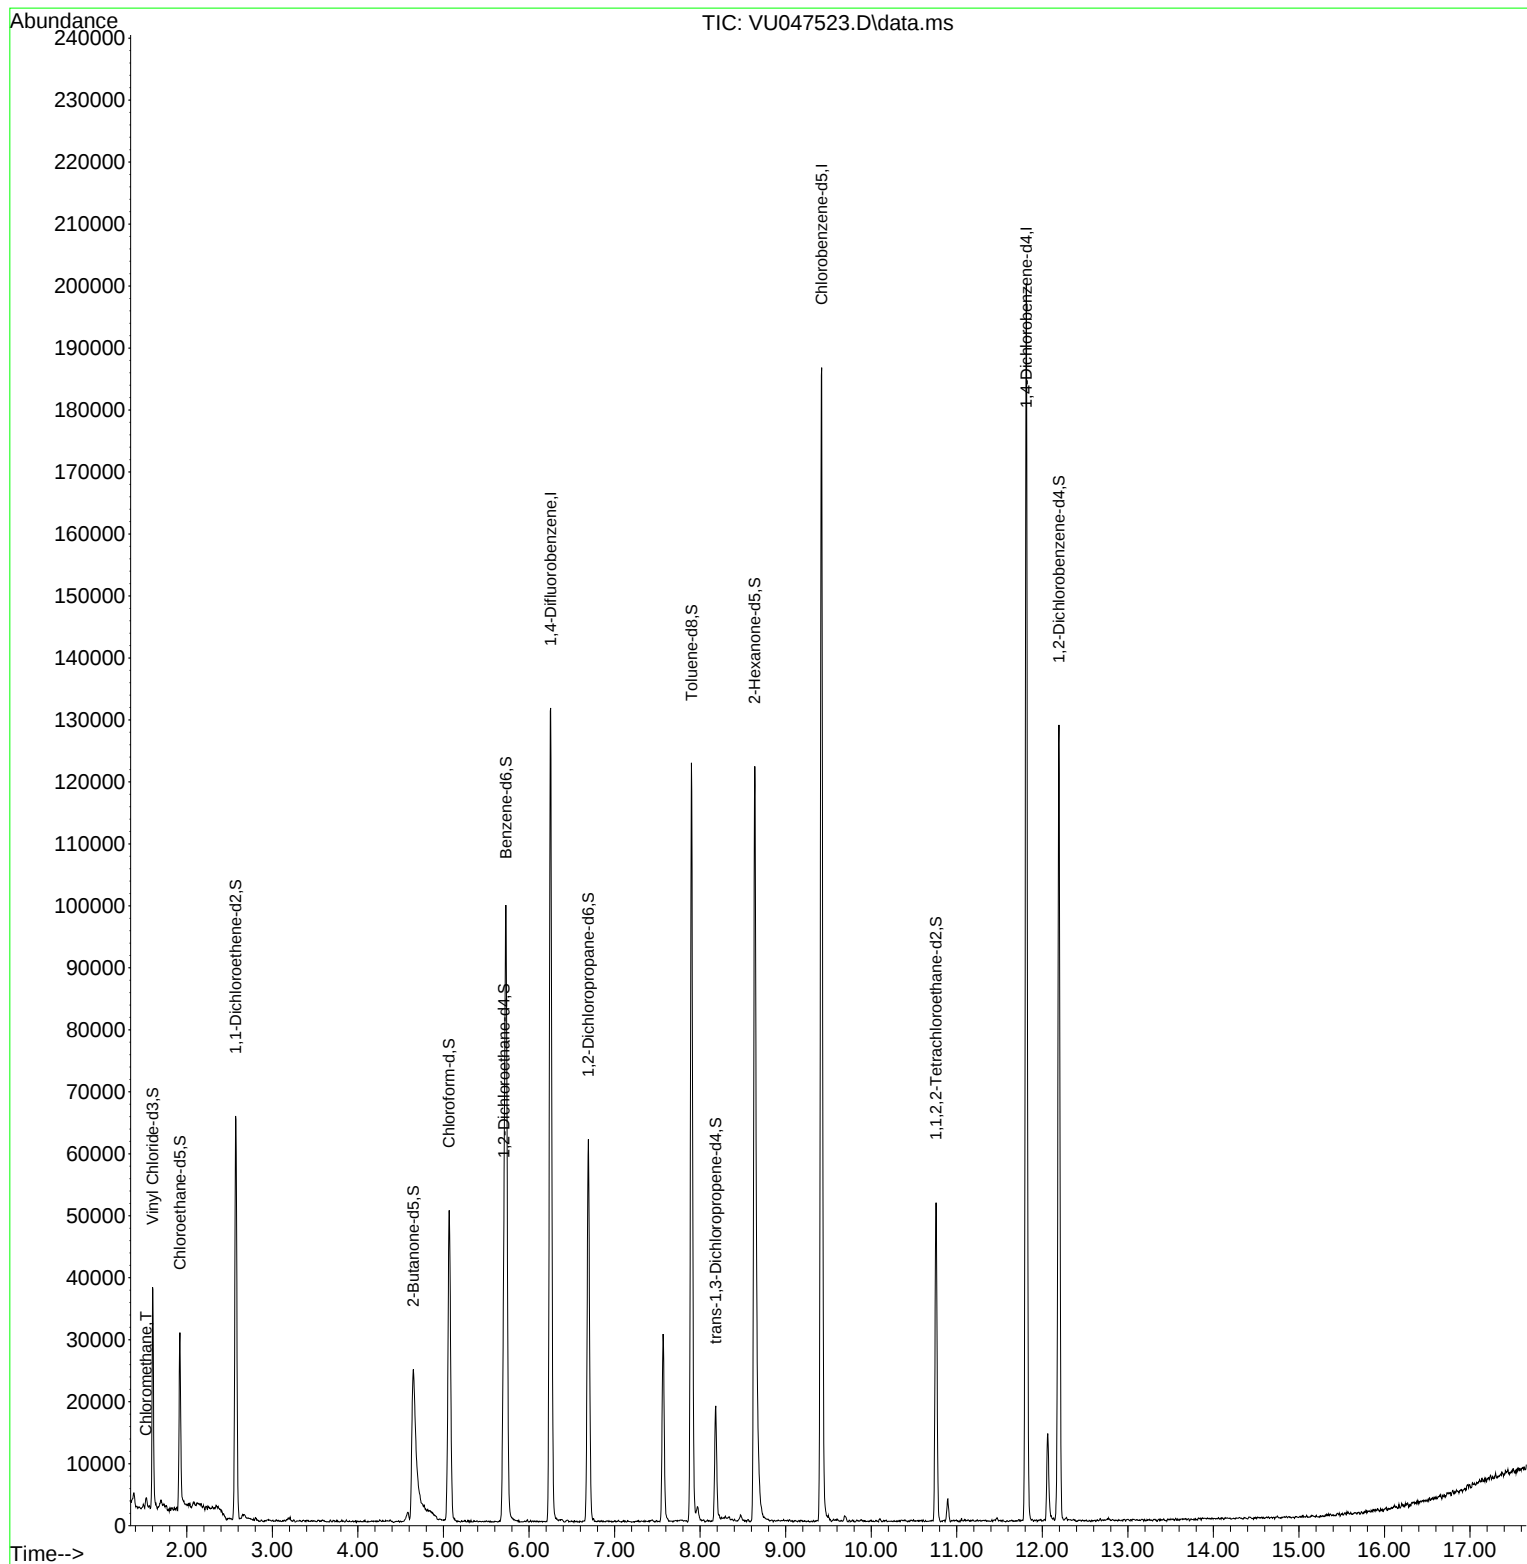

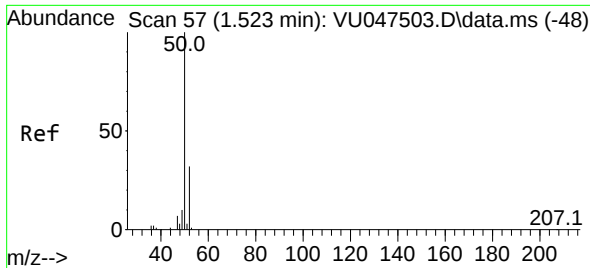

#3
Chloromethane
Concen: 0.163 ug/L
RT: 1.523 min Scan# 51
Delta R.T. 0.000 min
Lab File: VU047523.D
Acq: 12 Mar 2022 03:48

Instrument :
MSVOA_U
ClientSampleId :
ETNK6

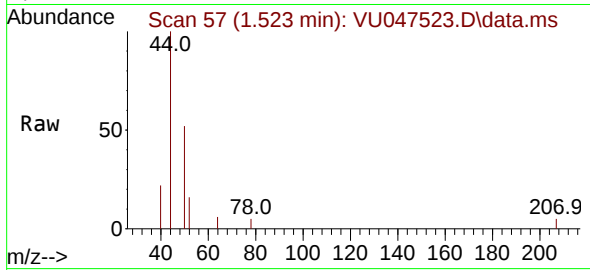

Tgt Ion: 50 Resp: 1382
Ion Ratio Lower Upper
50 100
52 31.5 22.5 41.9

