

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
 Data File : VU047514.D
 Acq On : 12 Mar 2022 00:16
 Operator : SY/MD
 Sample : N1906-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNM5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	93	rBV	38052	44283	14.85%	1.637%
2	1.919	171	180	198	rBV	29562	41177	13.81%	1.522%
3	2.572	372	383	398	rVB	68841	111747	37.47%	4.130%
4	4.645	1014	1028	1061	rBV	27208	101304	33.97%	3.744%
5	5.067	1140	1159	1189	rBV2	64010	155046	51.99%	5.731%
6	5.729	1344	1365	1386	rBV2	104800	265582	89.05%	9.816%
7	6.250	1514	1527	1548	rBV	123388	236053	79.15%	8.725%
8	6.694	1651	1665	1684	rBV	62014	121155	40.62%	4.478%
9	7.568	1925	1937	1957	rBV	33266	57212	19.18%	2.115%
10	7.899	2028	2040	2053	rBV	129152	221399	74.24%	8.183%
11	7.970	2053	2062	2079	rVB	69050	120566	40.43%	4.456%
12	8.182	2118	2128	2140	rBV2	19580	34325	11.51%	1.269%
13	8.475	2208	2219	2229	rBV3	1788	3111	1.04%	0.115%
14	8.639	2257	2270	2299	rBV	135924	272742	91.45%	10.081%
15	9.417	2499	2512	2531	rBV	174894	298235	100.00%	11.023%
16	9.504	2532	2539	2549	rVB2	5299	7350	2.46%	0.272%
17	10.758	2917	2929	2942	rBV2	55203	88099	29.54%	3.256%
18	10.893	2961	2971	2984	rBV	5524	9398	3.15%	0.347%
19	11.812	3246	3257	3275	rVB	185449	294337	98.69%	10.879%
20	12.063	3328	3335	3344	rBV4	3779	6235	2.09%	0.230%
21	12.195	3364	3376	3393	rBV	132368	216143	72.47%	7.989%




Sum of corrected areas: 2705499

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
Data File : VU047514.D
Acq On : 12 Mar 2022 00:16
Operator : SY/MD
Sample : N1906-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

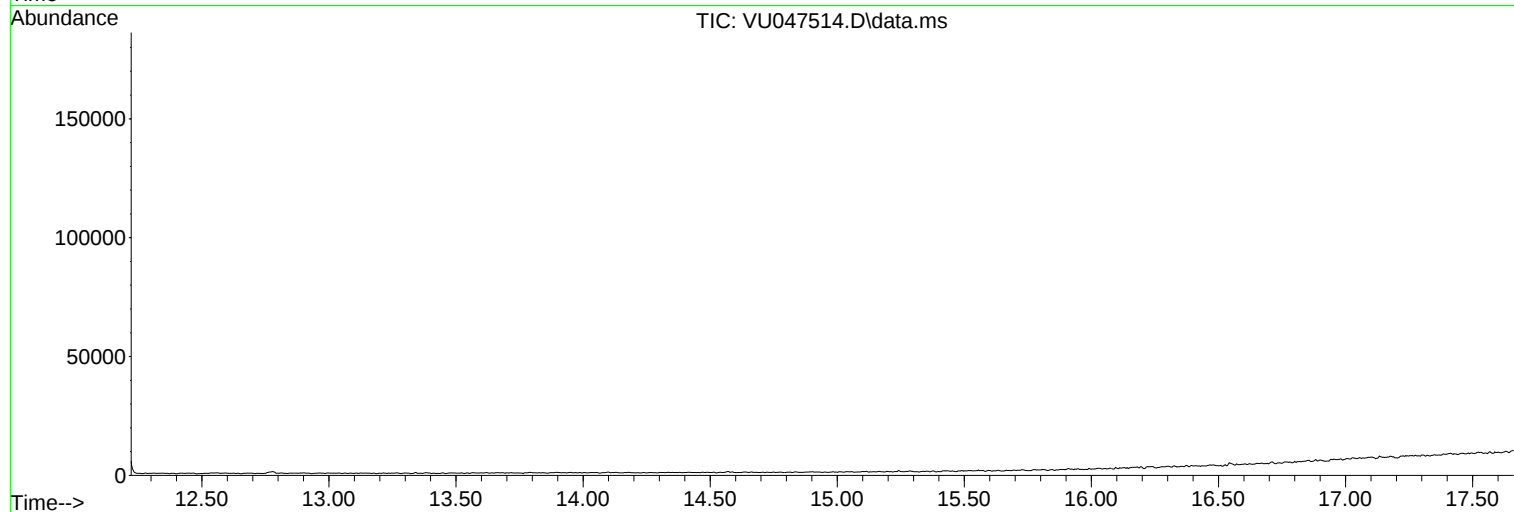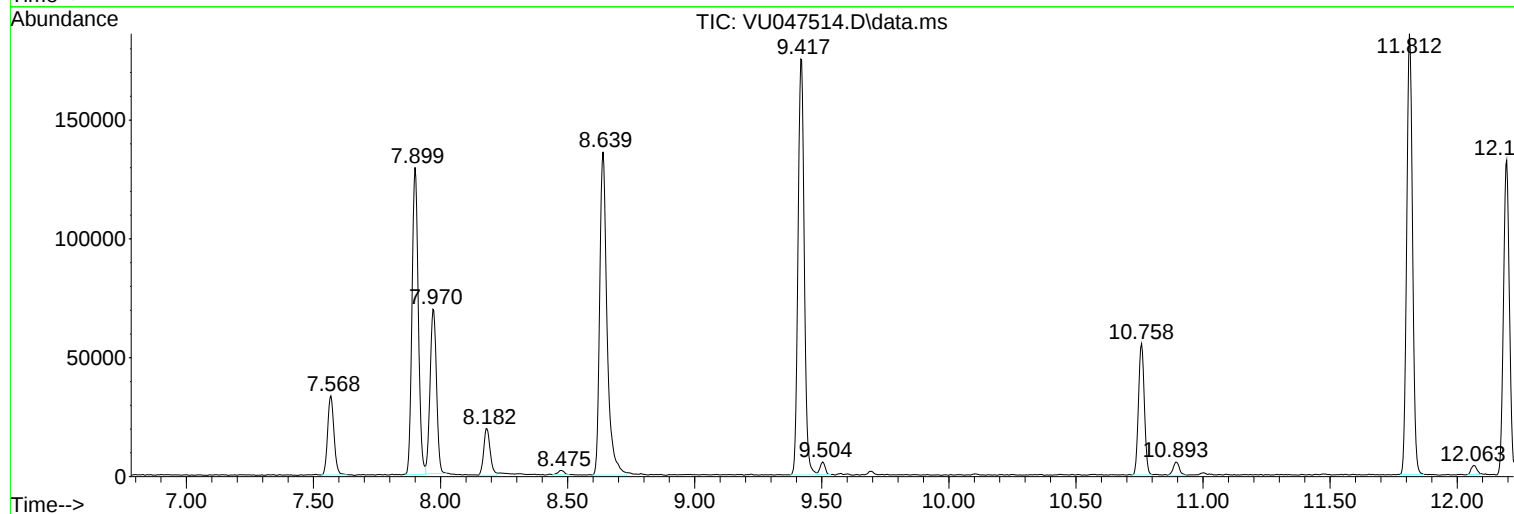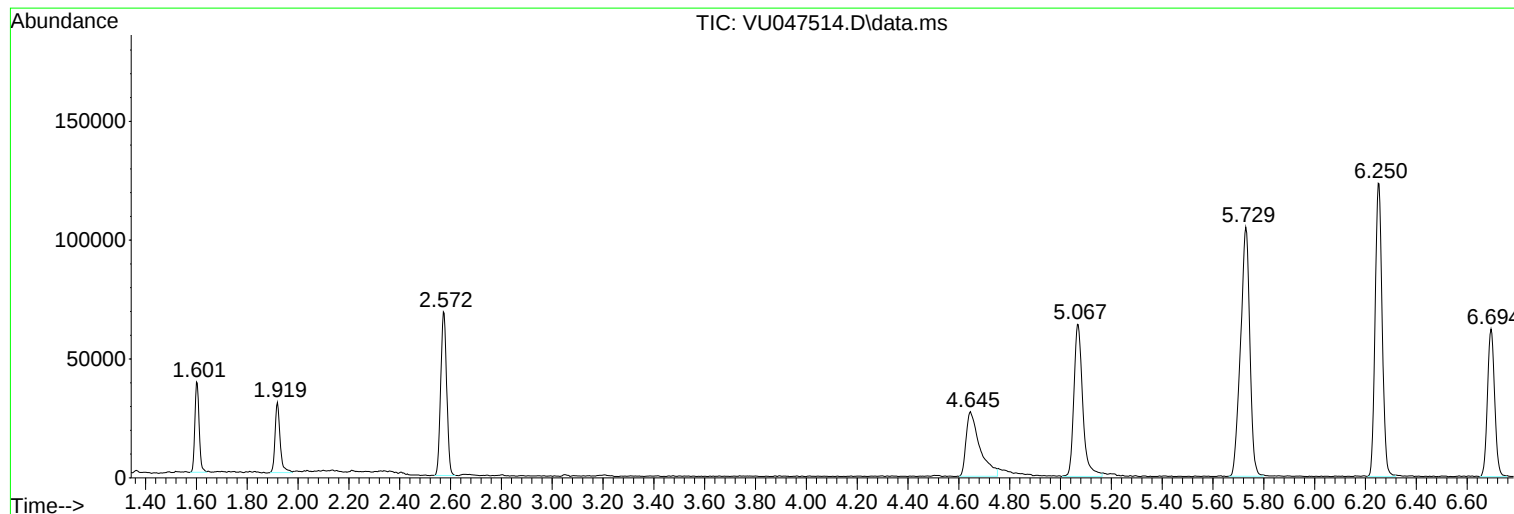

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
Data File : VU047514.D
Acq On : 12 Mar 2022 00:16
Operator : SY/MD
Sample : N1906-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
Data File : VU047514.D
Acq On : 12 Mar 2022 00:16
Operator : SY/MD
Sample : N1906-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc