

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
 Data File : VU047516.D
 Acq On : 12 Mar 2022 01:03
 Operator : SY/MD
 Sample : N1861-23
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YATN3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	95	rVB	39374	46838	14.00%	1.628%
2	1.919	172	180	191	rBV	30024	41027	12.27%	1.426%
3	2.572	372	383	399	rVB	70060	114184	34.14%	3.968%
4	2.658	399	410	421	rBV	3118	8031	2.40%	0.279%
5	4.649	1014	1029	1068	rBV	26197	102792	30.74%	3.572%
6	5.070	1144	1160	1187	rVB2	56005	142594	42.64%	4.956%
7	5.391	1247	1260	1275	rBV3	12156	26705	7.98%	0.928%
8	5.729	1344	1365	1390	rBV2	104859	269078	80.46%	9.351%
9	6.253	1514	1528	1548	rBV	138212	262325	78.44%	9.117%
10	6.546	1605	1619	1633	rBV2	79402	149662	44.75%	5.201%
11	6.694	1651	1665	1684	rBV	63772	123947	37.06%	4.308%
12	7.568	1925	1937	1952	rBV	32727	57691	17.25%	2.005%
13	7.899	2028	2040	2058	rBV	132068	227569	68.04%	7.909%
14	8.182	2118	2128	2141	rBV2	19655	33454	10.00%	1.163%
15	8.639	2258	2270	2299	rBV	134503	274468	82.07%	9.539%
16	9.417	2497	2512	2537	rBV	196573	332842	99.52%	11.567%
17	10.758	2916	2929	2943	rBV	55205	88355	26.42%	3.071%
18	10.893	2964	2971	2984	rVB2	3907	5868	1.75%	0.204%
19	11.812	3243	3257	3274	rBV	215685	334443	100.00%	11.623%
20	12.063	3324	3335	3349	rBV2	10311	16908	5.06%	0.588%
21	12.195	3364	3376	3392	rVB	134694	218649	65.38%	7.599%




Sum of corrected areas: 2877430

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
Data File : VU047516.D
Acq On : 12 Mar 2022 01:03
Operator : SY/MD
Sample : N1861-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YATN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

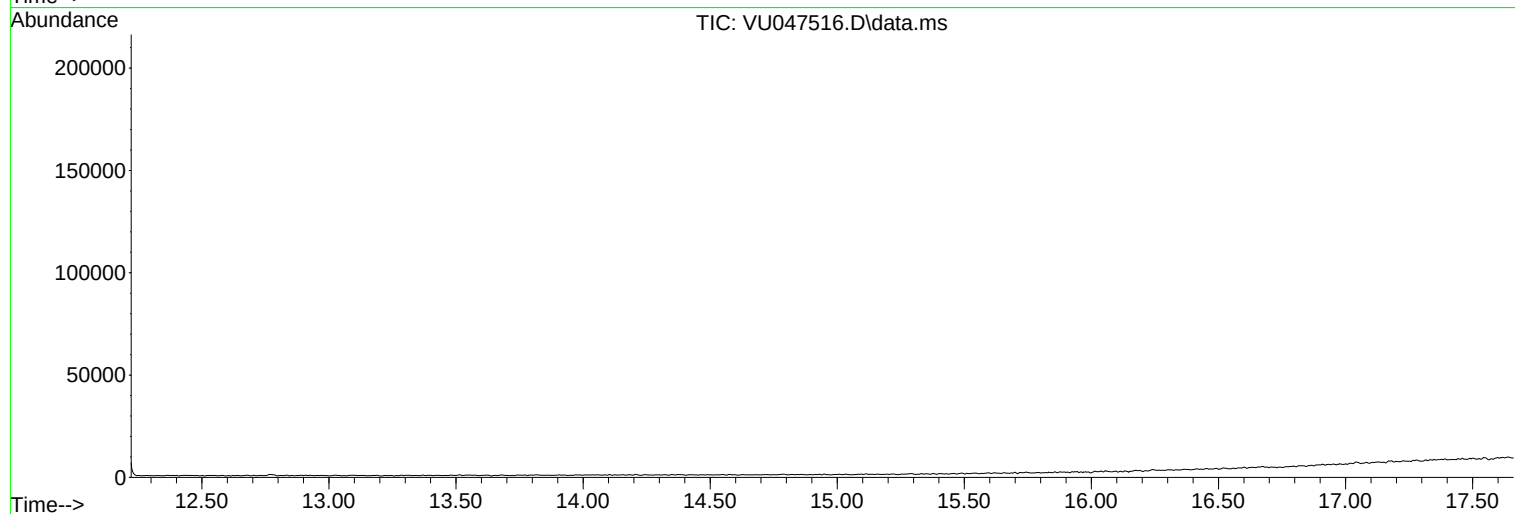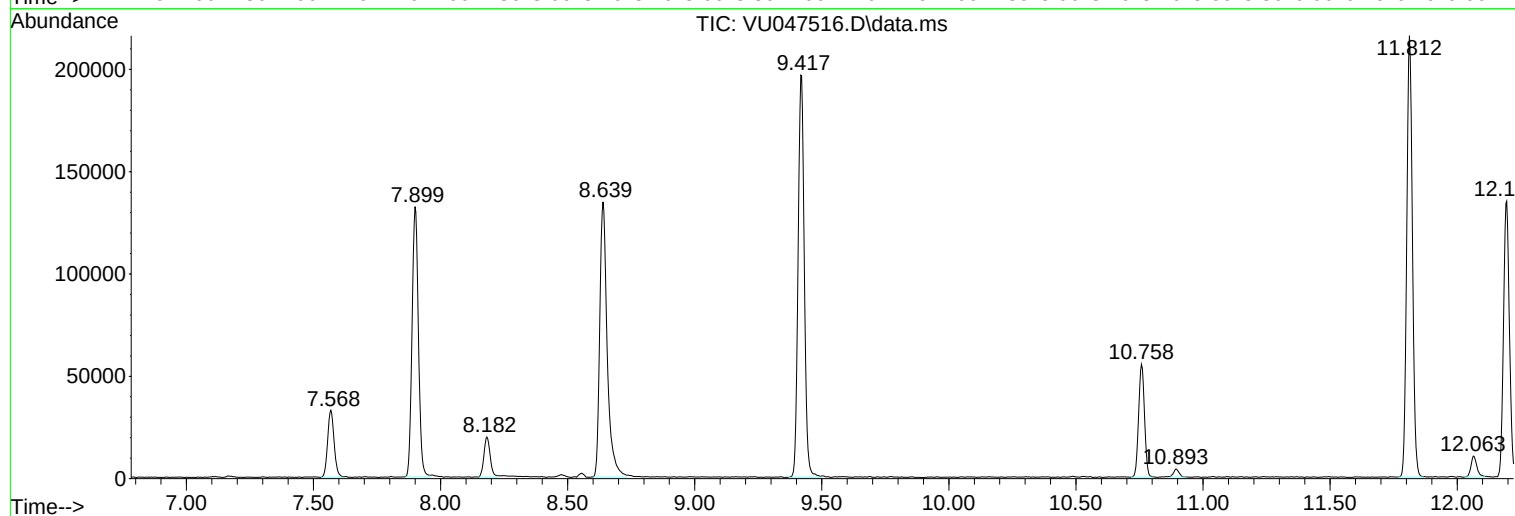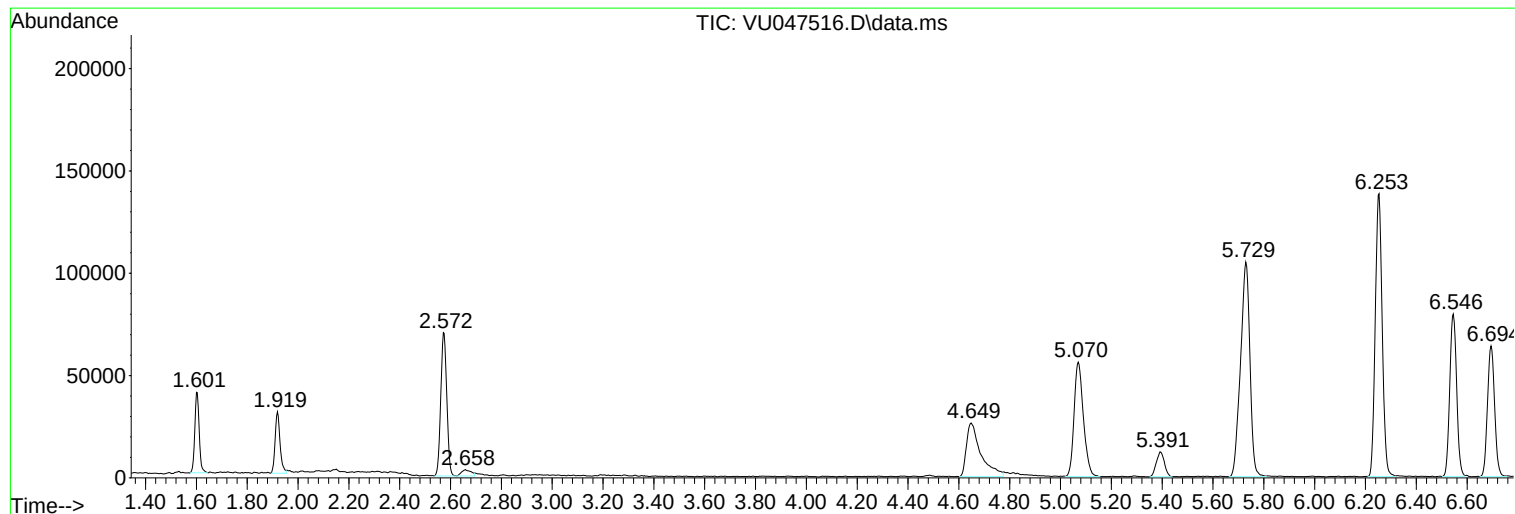

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
Data File : VU047516.D
Acq On : 12 Mar 2022 01:03
Operator : SY/MD
Sample : N1861-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YATN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
Data File : VU047516.D
Acq On : 12 Mar 2022 01:03
Operator : SY/MD
Sample : N1861-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YATN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
