

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
 Data File : VU047520.D
 Acq On : 12 Mar 2022 02:38
 Operator : SY/MD
 Sample : N1858-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNH2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU047520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	21	rVB2	6456	9832	3.16%	0.330%
2	1.607	72	83	103	rBV2	209373	253044	81.36%	8.496%
3	1.919	171	180	195	rBV	28942	39323	12.64%	1.320%
4	2.571	372	383	398	rBV	65363	107182	34.46%	3.599%
5	3.362	618	629	643	rBV2	10272	19554	6.29%	0.657%
6	4.671	1015	1036	1057	rBV3	112634	311004	100.00%	10.442%
7	5.067	1141	1159	1183	rVB2	50063	111561	35.87%	3.746%
8	5.729	1342	1365	1393	rBV2	102071	266641	85.74%	8.953%
9	6.253	1512	1528	1550	rBV	128679	243112	78.17%	8.163%
10	6.546	1612	1619	1628	rVB5	2628	4353	1.40%	0.146%
11	6.693	1651	1665	1684	rBV	61568	119311	38.36%	4.006%
12	7.568	1926	1937	1952	rBV	31266	54820	17.63%	1.841%
13	7.899	2028	2040	2058	rBV	125987	216586	69.64%	7.272%
14	8.182	2117	2128	2141	rBV2	18548	32153	10.34%	1.080%
15	8.639	2258	2270	2303	rBV	132074	272901	87.75%	9.163%
16	9.417	2500	2512	2532	rBV	181855	304119	97.79%	10.211%
17	10.758	2917	2929	2945	rVB	54156	86133	27.70%	2.892%
18	10.893	2962	2971	2979	rBV2	2661	4305	1.38%	0.145%
19	11.812	3244	3257	3274	rBV	193506	308576	99.22%	10.361%
20	12.063	3327	3335	3346	rVB2	3463	5503	1.77%	0.185%
21	12.195	3364	3376	3392	rBV	127519	208312	66.98%	6.994%




Sum of corrected areas: 2978325

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
Data File : VU047520.D
Acq On : 12 Mar 2022 02:38
Operator : SY/MD
Sample : N1858-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

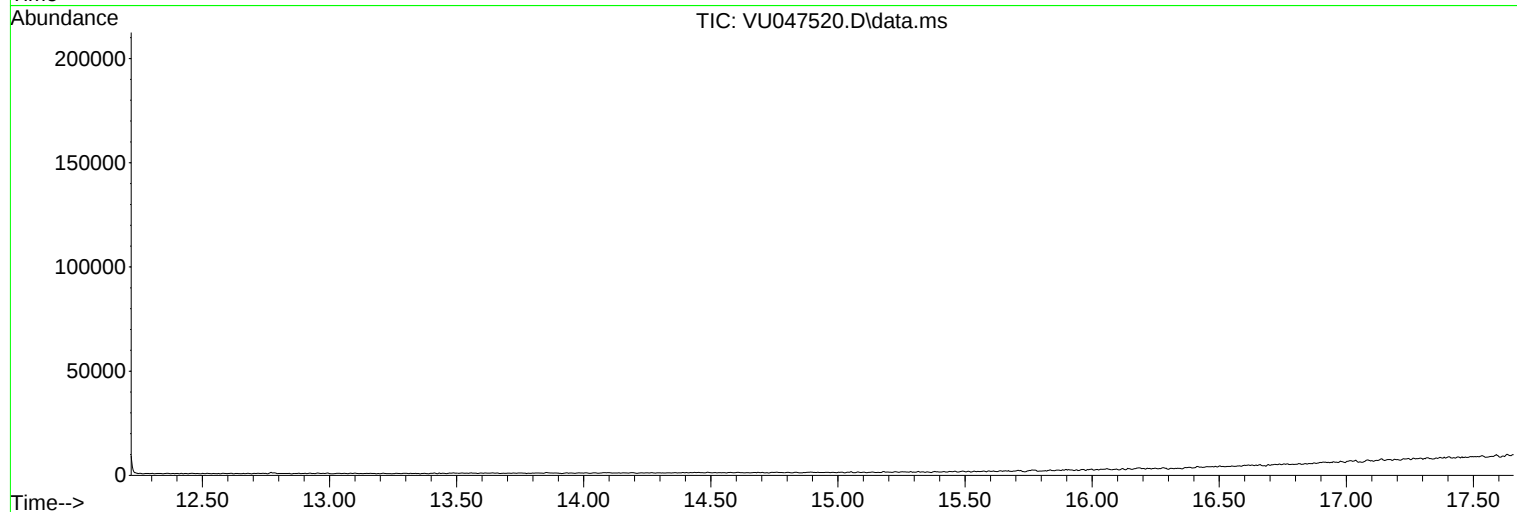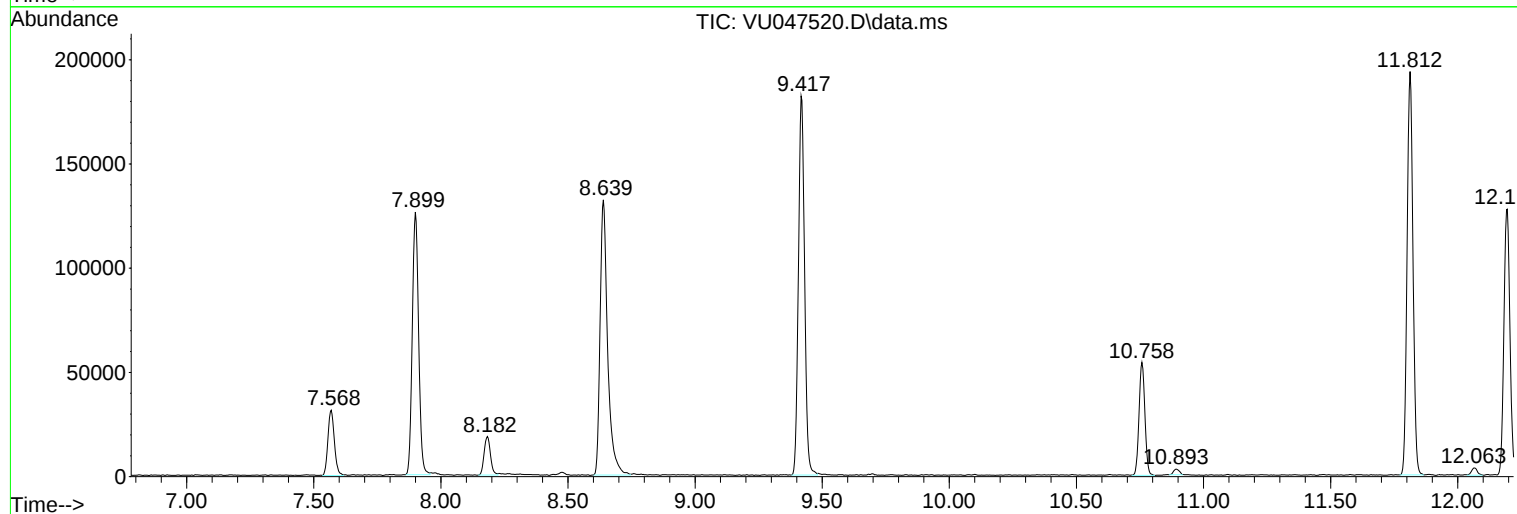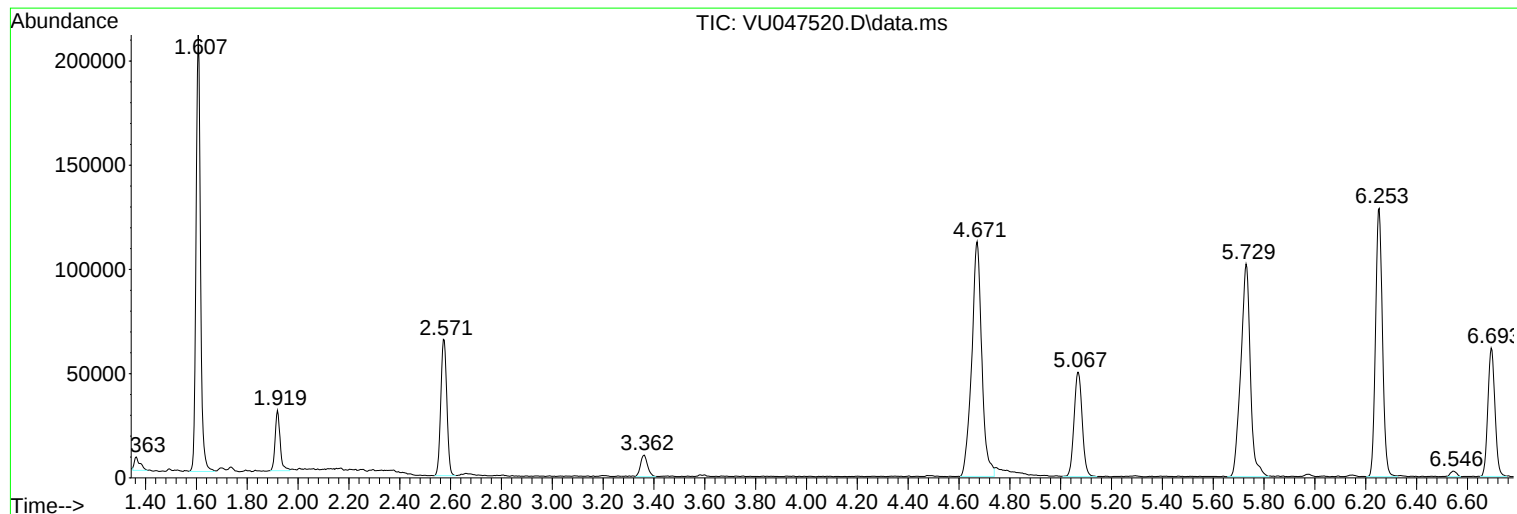

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
Data File : VU047520.D
Acq On : 12 Mar 2022 02:38
Operator : SY/MD
Sample : N1858-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
Data File : VU047520.D
Acq On : 12 Mar 2022 02:38
Operator : SY/MD
Sample : N1858-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc