

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
 Data File : VU047523.D
 Acq On : 12 Mar 2022 03:48
 Operator : SY/MD
 Sample : N1858-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNK6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	92	rBV	35690	41126	12.86%	1.629%
2	1.919	172	180	194	rBV	28745	40500	12.67%	1.604%
3	2.571	370	383	397	rBV	65164	106277	33.24%	4.209%
4	4.584	990	1009	1015	rBV	1502	3254	1.02%	0.129%
5	4.649	1015	1029	1066	rBV	24181	89143	27.88%	3.531%
6	5.067	1144	1159	1178	rBV	49945	107168	33.52%	4.245%
7	5.729	1344	1365	1387	rBV3	99465	254482	79.60%	10.079%
8	6.253	1514	1528	1548	rBV	131273	249301	77.98%	9.874%
9	6.693	1652	1665	1680	rBV2	61570	116646	36.49%	4.620%
10	7.568	1925	1937	1954	rBV2	30324	53333	16.68%	2.112%
11	7.899	2025	2040	2055	rBV	122512	212320	66.41%	8.409%
12	7.967	2056	2061	2072	rVB3	2172	3934	1.23%	0.156%
13	8.182	2117	2128	2139	rBV	18584	30890	9.66%	1.223%
14	8.639	2254	2270	2302	rBV	121898	257382	80.51%	10.194%
15	9.420	2500	2513	2531	rBV	186073	314230	98.29%	12.446%
16	10.758	2918	2929	2945	rVB	51505	83767	26.20%	3.318%
17	10.896	2962	2972	2981	rVB	3690	5637	1.76%	0.223%
18	11.812	3245	3257	3276	rBV	199559	319705	100.00%	12.662%
19	12.063	3326	3335	3346	rBV2	14043	23432	7.33%	0.928%
20	12.195	3360	3376	3393	rBV	128353	212306	66.41%	8.409%




Sum of corrected areas: 2524833

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
Data File : VU047523.D
Acq On : 12 Mar 2022 03:48
Operator : SY/MD
Sample : N1858-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

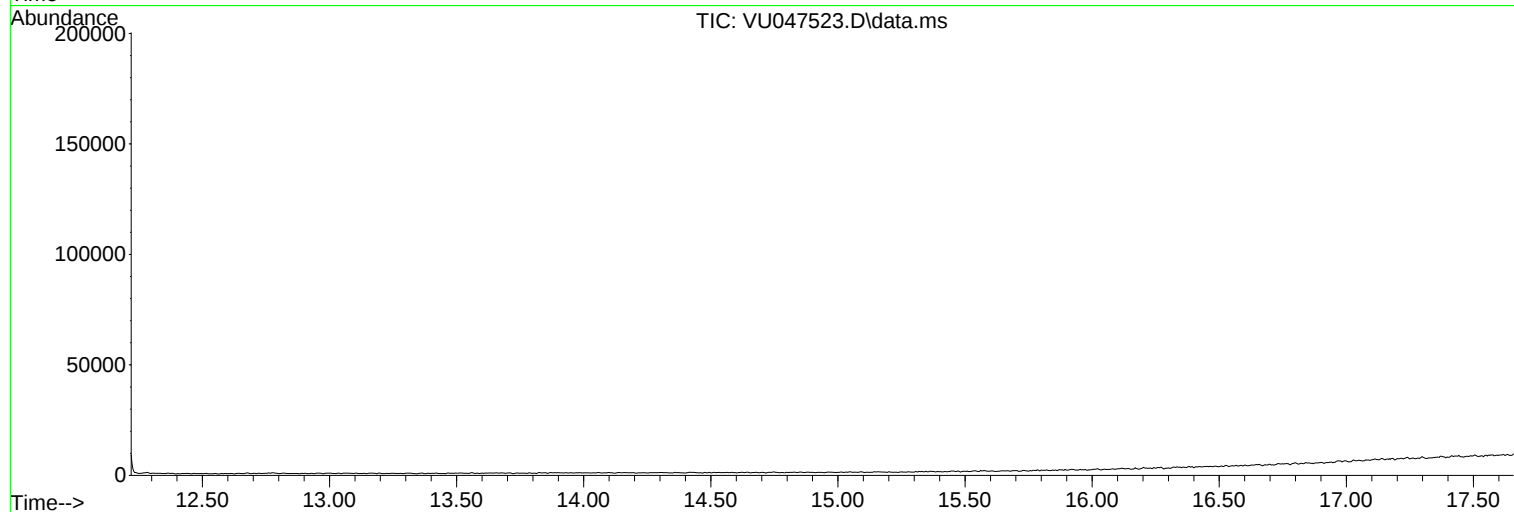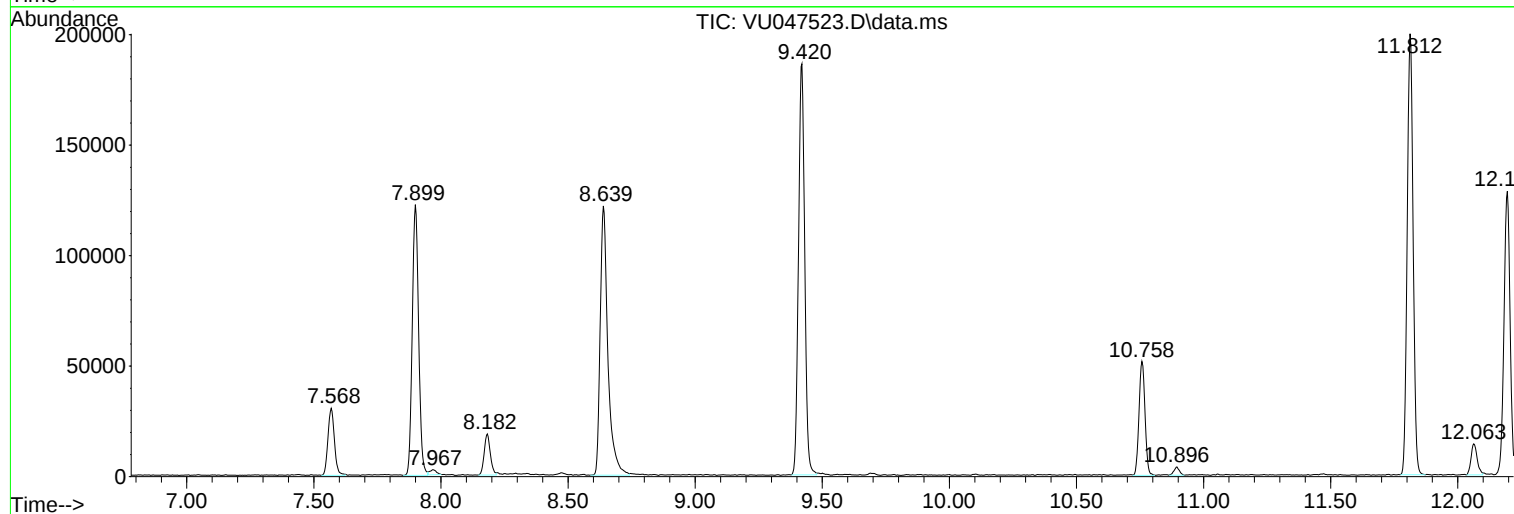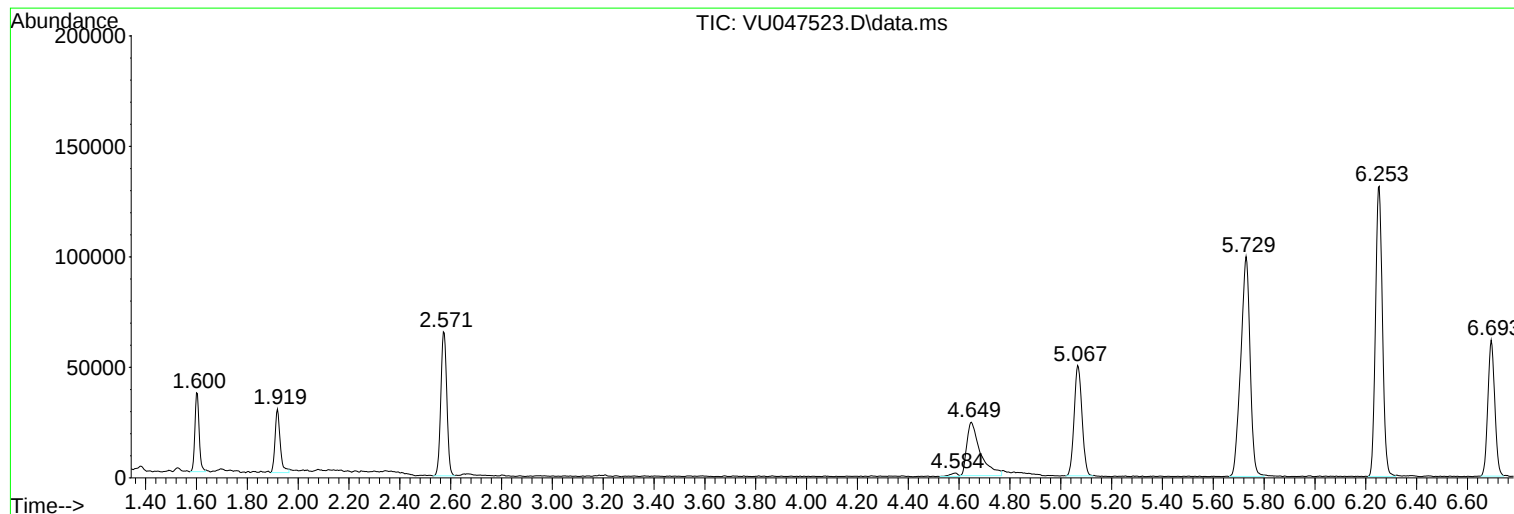

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
Data File : VU047523.D
Acq On : 12 Mar 2022 03:48
Operator : SY/MD
Sample : N1858-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
Data File : VU047523.D
Acq On : 12 Mar 2022 03:48
Operator : SY/MD
Sample : N1858-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc