
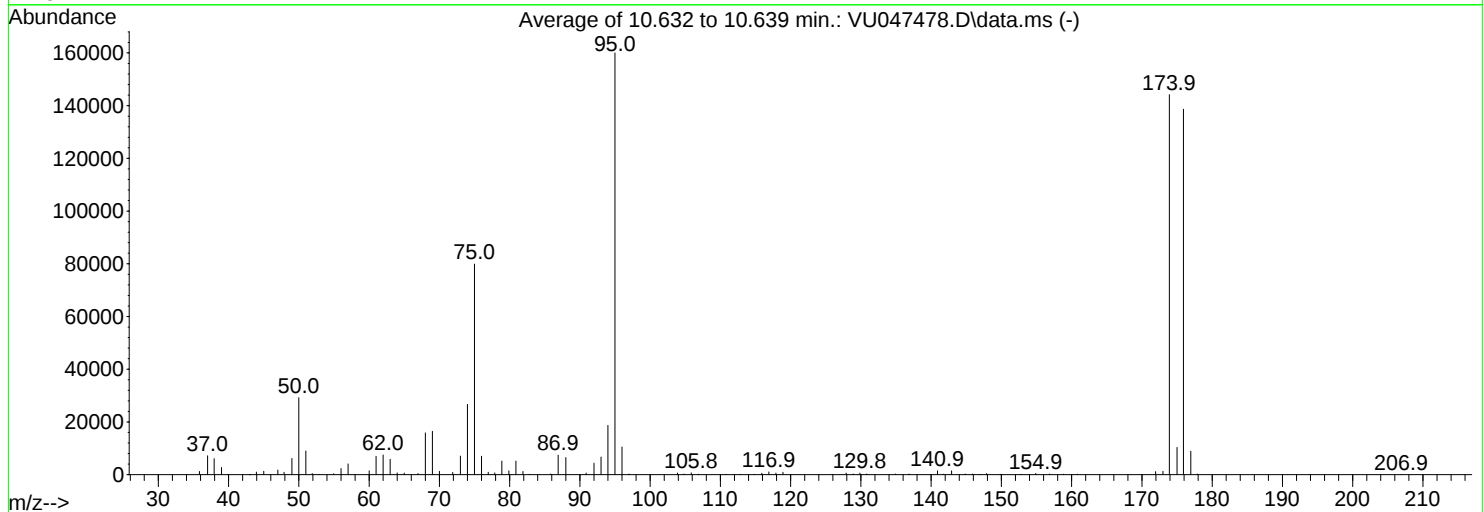


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031122\
Data File : VU047478.D
Acq On : 11 Mar 2022 08:48
Operator : SY/MD
Sample : BFB066
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB066

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030922WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Mar 14 12:06:39 2022

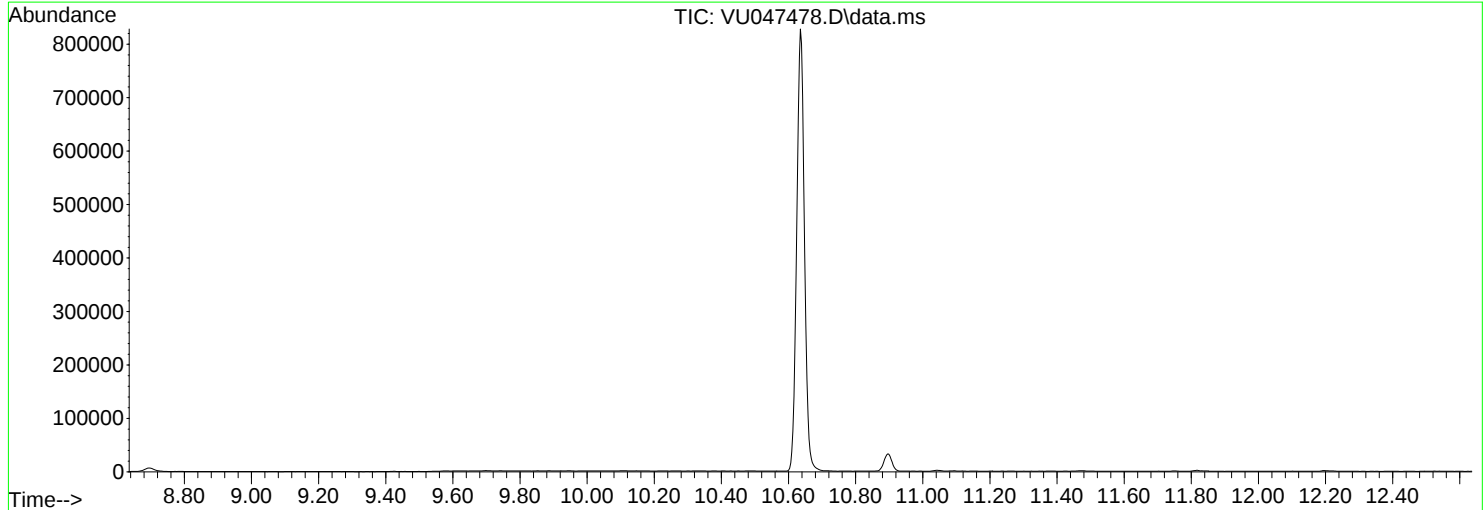

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	29227	PASS
75	95	30	80	49.9	79915	PASS
95	95	100	100	100.0	160043	PASS
96	95	5	9	6.6	10508	PASS
173	174	0.00	2	0.9	1306	PASS
174	95	50	120	90.1	144192	PASS
175	174	5	9	7.2	10339	PASS
176	174	95	101	96.1	138637	PASS
177	176	5	9	6.4	8884	PASS

m/z	Abundance
35.90	771.0
37.90	216.0
39.90	250.0
43.90	228.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066

m/z	Abundance
35.90	1912.0
37.00	7160.0
38.00	6403.0
39.00	2852.0
39.90	327.0
44.00	1197.0
45.00	1307.0
47.00	1691.0
47.90	932.0
49.00	6164.0
50.00	28808.0
51.00	8903.0
51.90	400.0
54.90	406.0
56.00	2254.0
57.00	4033.0
57.90	170.0
60.00	1420.0
61.00	6913.0
62.00	7550.0
63.00	5974.0
64.00	688.0
65.00	582.0
67.00	454.0
68.00	15427.0
69.00	16143.0
70.00	1243.0
71.90	848.0
73.00	6948.0
74.00	26160.0
75.00	79040.0
76.00	6872.0
77.00	923.0
77.90	634.0
78.90	5079.0
79.90	1428.0
80.90	4970.0
81.90	1211.0
82.90	142.0
85.80	211.0
86.90	7204.0
88.00	6256.0
90.90	548.0
92.00	4359.0
93.00	6365.0
94.00	18272.0
95.00	155520.0
96.00	10612.0
97.00	270.0
103.90	705.0
104.80	201.0
105.80	630.0
106.90	170.0
110.80	127.0
112.90	135.0
114.80	177.0
115.90	546.0
116.90	955.0
117.90	637.0
118.90	842.0
123.90	109.0
125.90	102.0
127.90	549.0
128.90	257.0
129.90	571.0
130.80	230.0
135.00	224.0
136.80	232.0
140.90	1378.0
141.90	153.0
142.90	1412.0
144.90	261.0
145.90	226.0
147.00	115.0
147.90	429.0
149.80	116.0
152.80	123.0
154.90	403.0
156.80	247.0
158.80	167.0
160.90	214.0
171.90	1138.0
173.00	1316.0
173.90	137216.0
175.00	9854.0
175.90	130920.0
177.00	8629.0
177.90	285.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066

m/z	Abundance
35.90	2033.0
37.00	7412.0
38.00	6497.0
39.00	2797.0
39.90	298.0
44.00	1224.0
45.00	1285.0
45.90	108.0
47.00	1886.0
47.90	981.0
49.00	6294.0
50.00	30160.0
51.00	9296.0
51.90	435.0
52.90	104.0
55.00	398.0
56.00	2396.0
57.00	4188.0
57.90	147.0
60.00	1514.0
61.00	7122.0
62.00	7749.0
63.00	6010.0
64.00	683.0
65.00	615.0
66.90	410.0
68.00	16416.0
69.00	16960.0
70.00	1328.0
71.90	870.0
73.00	7217.0
74.00	27496.0
75.00	82648.0
76.00	7234.0
77.00	955.0
77.90	702.0
78.90	5331.0
79.90	1506.0
80.90	5383.0
81.90	1281.0
82.80	160.0
85.90	234.0
86.90	7666.0
88.00	6713.0
90.90	611.0
92.00	4538.0
93.00	6963.0
94.00	19248.0
95.00	165376.0
96.00	10959.0
97.00	272.0
103.90	639.0
104.80	212.0
105.80	707.0
106.90	174.0
110.80	138.0
112.80	141.0
114.80	149.0
115.90	565.0
116.90	1073.0
117.90	639.0
118.90	921.0
125.90	108.0
127.90	608.0
128.90	266.0
129.80	660.0
130.90	232.0
135.00	244.0
136.90	271.0
140.00	126.0
140.90	1545.0
141.80	164.0
142.90	1536.0
144.80	237.0
145.90	239.0
147.00	108.0
147.90	432.0
149.80	111.0
152.80	135.0
154.90	507.0
156.90	265.0
158.90	193.0
160.80	198.0
171.90	1169.0
173.00	1323.0
173.90	148608.0
175.00	10666.0
175.90	143296.0
177.00	9119.0
177.90	281.0
207.00	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066

m/z	Abundance
35.90	2006.0
37.00	7003.0
38.00	6005.0
39.00	2529.0
39.90	279.0
43.00	110.0
44.00	1157.0
45.00	1205.0
45.90	116.0
47.00	1787.0
47.90	900.0
49.00	5870.0
50.00	28712.0
51.00	8829.0
51.90	437.0
52.90	115.0
55.00	385.0
56.00	2329.0
57.00	4010.0
58.00	136.0
60.00	1469.0
61.00	6711.0
62.00	7189.0
63.00	5494.0
64.00	643.0
65.00	639.0
66.90	365.0
68.00	15769.0
69.00	16238.0
70.00	1281.0
71.90	792.0
73.00	6884.0
74.00	26336.0
75.00	78056.0
76.00	6779.0
76.90	891.0
77.90	667.0
78.90	5056.0
79.90	1450.0
80.90	5200.0
81.90	1232.0
82.90	174.0
85.90	238.0
86.90	7311.0
88.00	6628.0
90.90	636.0
92.00	4232.0
93.00	6710.0
94.00	18608.0
95.00	159232.0
96.00	9952.0
97.00	243.0
103.90	555.0
104.80	235.0
105.90	713.0
106.90	160.0
110.80	119.0
112.80	139.0
114.90	139.0
115.90	525.0
116.90	1094.0
117.90	562.0
118.90	922.0
125.90	113.0
127.90	599.0
128.90	260.0
129.80	656.0
130.90	196.0
134.90	263.0
136.90	294.0
139.90	128.0
140.90	1548.0
141.70	182.0
142.90	1516.0
144.80	217.0
145.90	241.0
147.90	392.0
149.80	103.0
152.80	119.0
154.90	504.0
156.90	281.0
158.90	209.0
160.80	177.0
172.00	1141.0
173.00	1280.0
173.90	146752.0
175.00	10497.0
175.90	141696.0
176.90	8904.0
177.90	231.0
206.90	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066