

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031124\
 Data File : VU058031.D
 Acq On : 11 Mar 2024 10:24
 Operator : MD/SY
 Sample : VU0311WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK144

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU058031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	86	94	105	rVB	58823	65207	13.50%	1.685%
2	1.904	182	191	206	rVB	54448	69737	14.44%	1.802%
3	2.557	383	394	412	rBV	96725	157596	32.63%	4.073%
4	3.036	532	543	553	rBV3	4031	7691	1.59%	0.199%
5	4.615	1024	1034	1071	rBV	52033	142397	29.48%	3.680%
6	5.052	1154	1170	1190	rBV	94201	211911	43.87%	5.477%
7	5.718	1358	1377	1405	rBV2	185670	483046	100.00%	12.485%
8	6.242	1527	1540	1568	rBV	171773	338286	70.03%	8.743%
9	6.682	1664	1677	1696	rBV	116132	230483	47.71%	5.957%
10	7.560	1939	1950	1969	rBV	50867	94539	19.57%	2.443%
11	7.891	2040	2053	2074	rBV	224566	398561	82.51%	10.301%
12	8.177	2131	2142	2156	rBV	28624	50440	10.44%	1.304%
13	8.627	2270	2282	2321	rBV2	195646	403759	83.59%	10.436%
14	9.412	2514	2526	2554	rBV	235263	409904	84.86%	10.594%
15	10.750	2931	2942	2962	rBV2	69192	113774	23.55%	2.941%
16	11.807	3259	3271	3294	rBV	219225	371774	76.96%	9.609%
17	12.190	3377	3390	3417	rBV	179461	309058	63.98%	7.988%
18	12.766	3553	3569	3579	rBV3	3758	5865	1.21%	0.152%
19	13.849	3899	3906	3919	rVB5	2931	5037	1.04%	0.130%




Sum of corrected areas: 3869065

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031124\
Data File : VU058031.D
Acq On : 11 Mar 2024 10:24
Operator : MD/SY
Sample : VU0311WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK144

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

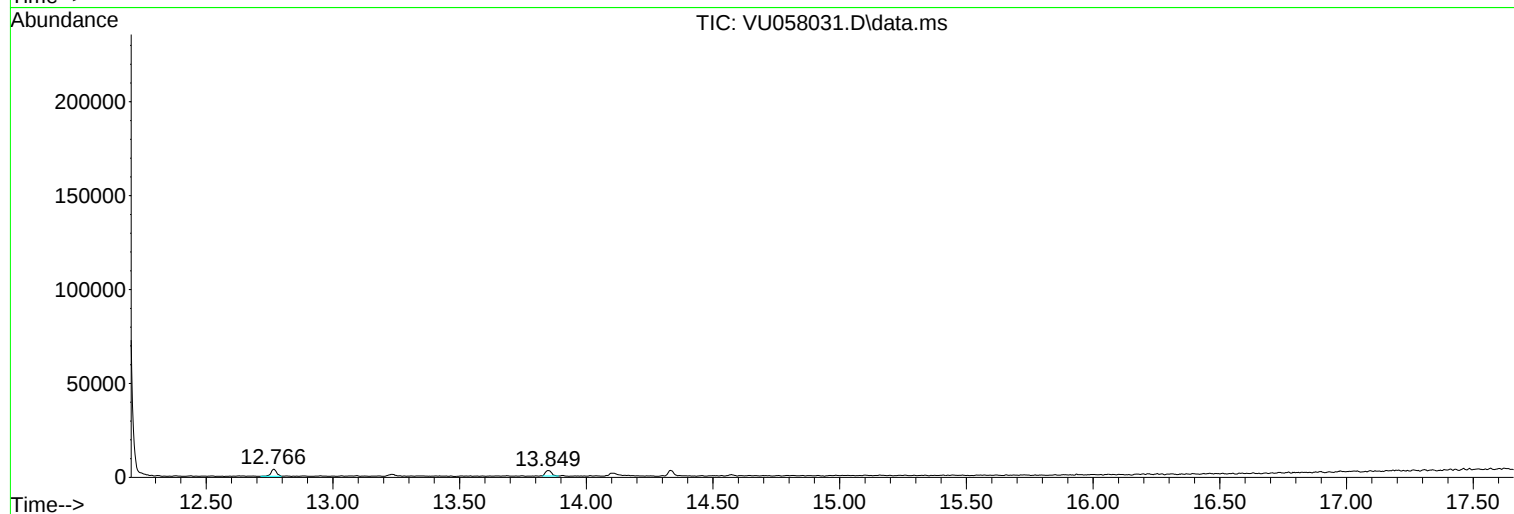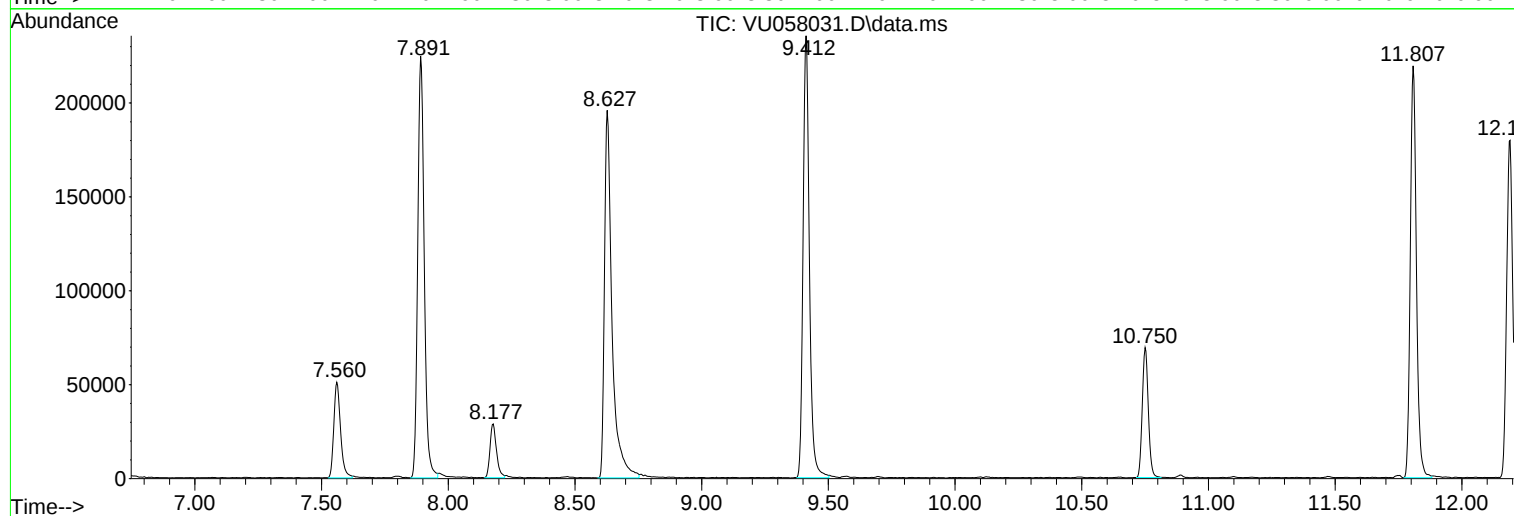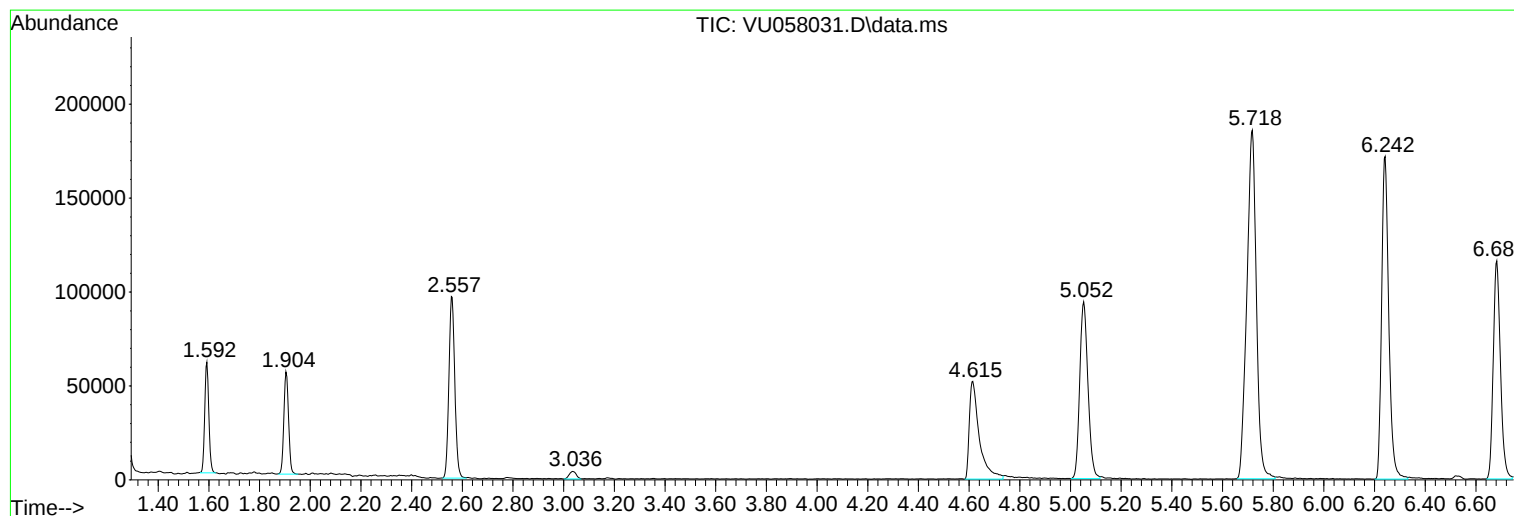

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031124\
Data File : VU058031.D
Acq On : 11 Mar 2024 10:24
Operator : MD/SY
Sample : VU0311WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK144

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031124\
Data File : VU058031.D
Acq On : 11 Mar 2024 10:24
Operator : MD/SY
Sample : VU0311WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK144

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------