

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031124\
 Data File : VU058034.D
 Acq On : 11 Mar 2024 11:44
 Operator : MD/SY
 Sample : P1636-22
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCNQ1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU058034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	87	94	111	rVB	61419	70717	13.77%	1.720%
2	1.908	183	192	204	rVB	57056	71710	13.96%	1.744%
3	2.560	381	395	410	rBV	100514	164699	32.06%	4.006%
4	2.789	456	466	480	rVB2	5345	9668	1.88%	0.235%
5	4.612	1023	1033	1063	rBV	58166	151677	29.53%	3.689%
6	5.052	1156	1170	1195	rBV	97962	224554	43.71%	5.462%
7	5.718	1357	1377	1407	rBV2	199958	513714	100.00%	12.496%
8	6.242	1528	1540	1564	rBV	173690	343109	66.79%	8.346%
9	6.682	1664	1677	1695	rBV	121255	242020	47.11%	5.887%
10	7.560	1939	1950	1975	rBV	53963	100222	19.51%	2.438%
11	7.891	2041	2053	2079	rBV	235366	424987	82.73%	10.337%
12	8.174	2129	2141	2171	rBV	30584	56680	11.03%	1.379%
13	8.547	2250	2257	2267	rBV3	7396	11711	2.28%	0.285%
14	8.628	2270	2282	2317	rBV2	199433	437154	85.10%	10.633%
15	9.412	2514	2526	2554	rBV	240790	422734	82.29%	10.283%
16	10.750	2931	2942	2961	rBV	75075	124309	24.20%	3.024%
17	10.891	2975	2986	2998	rVB3	4876	7946	1.55%	0.193%
18	11.807	3259	3271	3298	rBV	231784	388281	75.58%	9.445%
19	12.190	3378	3390	3412	rBV	202329	339129	66.02%	8.249%
20	12.769	3560	3570	3580	rBV2	3669	6117	1.19%	0.149%


Sum of corrected areas: 4111138

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031124\
Data File : VU058034.D
Acq On : 11 Mar 2024 11:44
Operator : MD/SY
Sample : P1636-22
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCNQ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

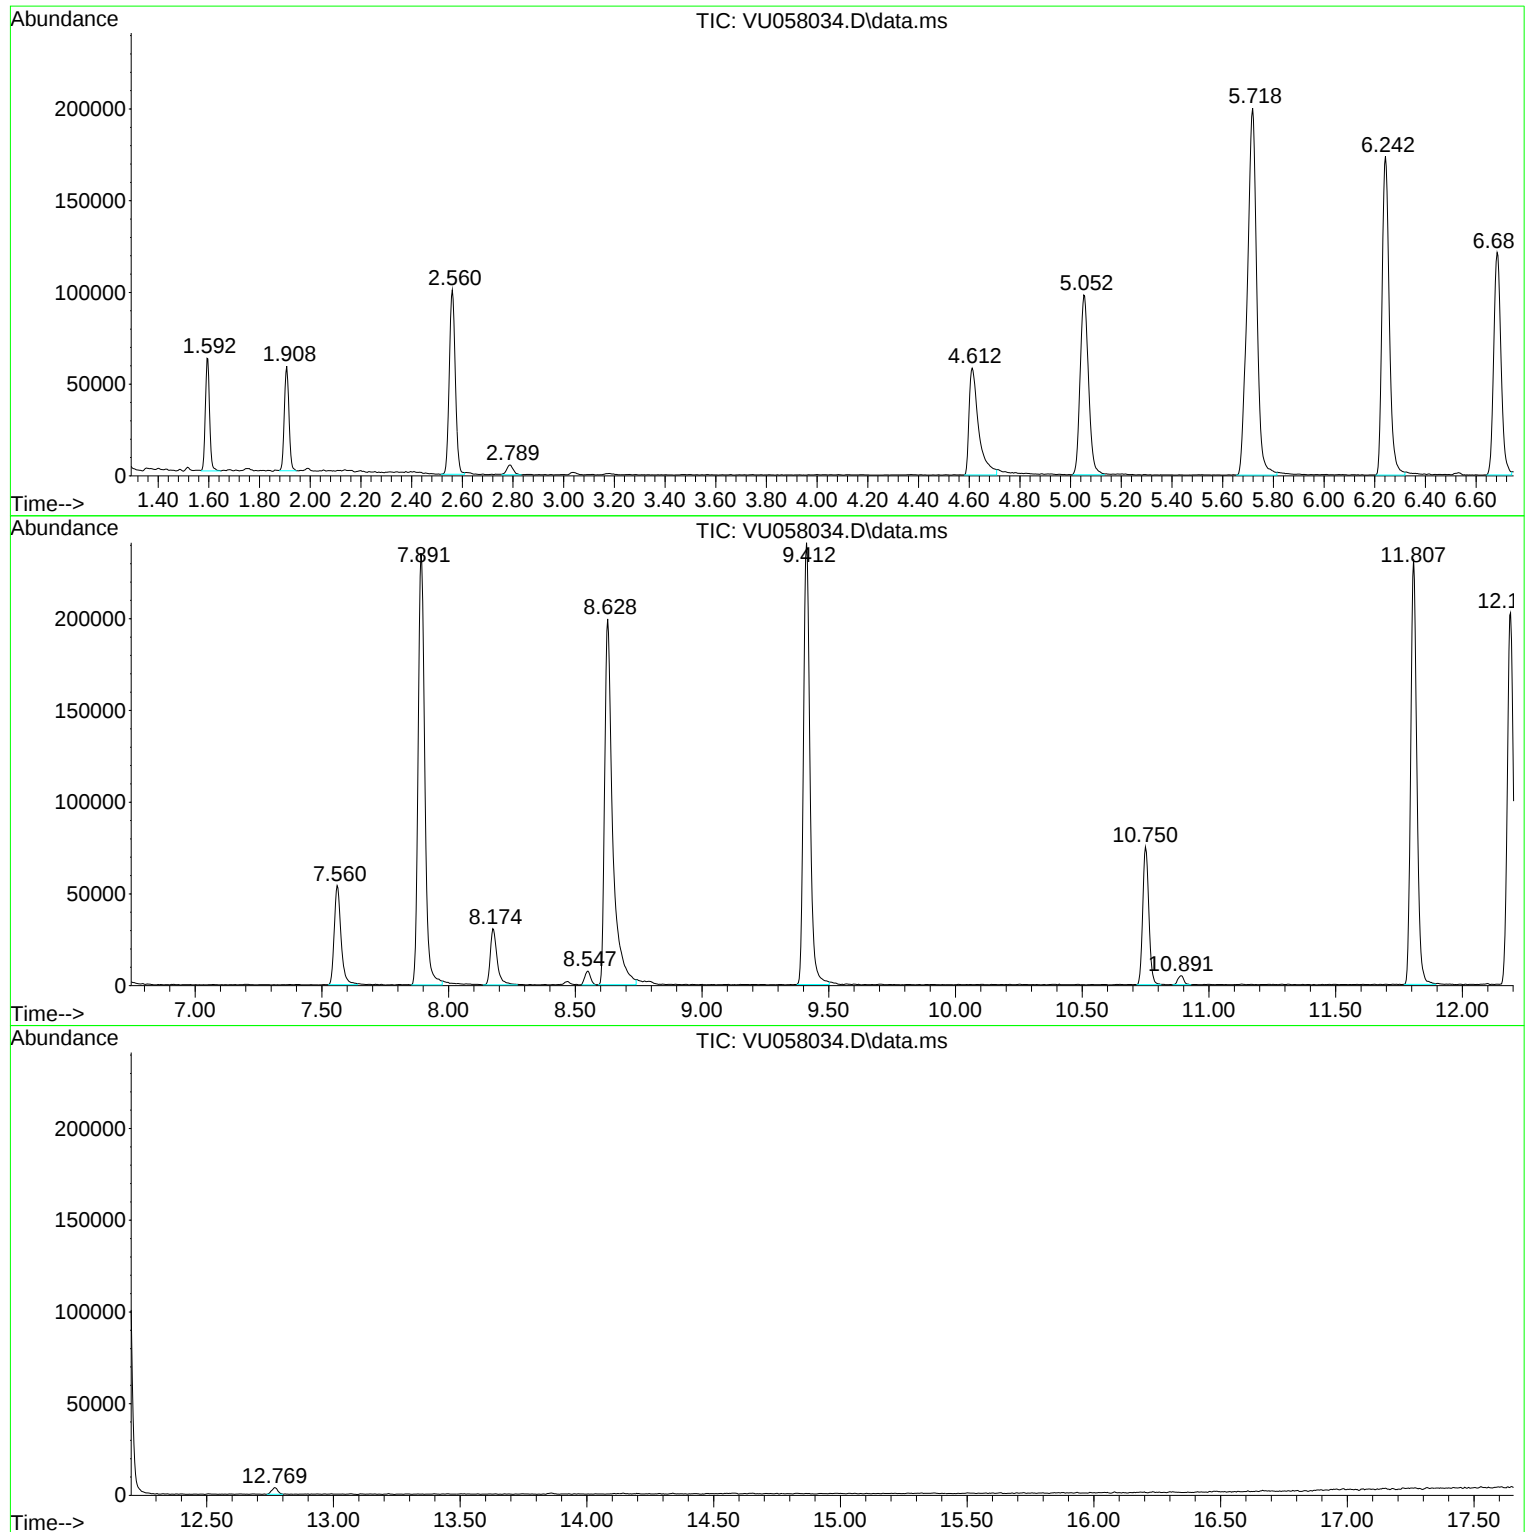

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031124\
Data File : VU058034.D
Acq On : 11 Mar 2024 11:44
Operator : MD/SY
Sample : P1636-22
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCNQ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031124\
Data File : VU058034.D
Acq On : 11 Mar 2024 11:44
Operator : MD/SY
Sample : P1636-22
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCNQ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc