

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031324\
 Data File : VU058077.D
 Acq On : 13 Mar 2024 13:36
 Operator : MD/SY
 Sample : P1741-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0GE9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU058077.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.467	50	55	65	rVB3	5963	7290	1.70%	0.197%
2	1.592	86	94	106	rVB	44021	51233	11.96%	1.383%
3	1.904	183	191	204	rVB	43646	55866	13.04%	1.508%
4	2.560	379	395	410	rBV	76474	124736	29.11%	3.368%
5	4.615	1023	1034	1070	rBV	54178	149430	34.88%	4.035%
6	5.052	1155	1170	1192	rBV	85672	195660	45.66%	5.283%
7	5.718	1358	1377	1401	rBV2	167410	428469	100.00%	11.569%
8	6.242	1525	1540	1563	rBV	169215	330250	77.08%	8.917%
9	6.682	1663	1677	1696	rBV	106455	210453	49.12%	5.682%
10	7.560	1940	1950	1972	rBV2	44339	81588	19.04%	2.203%
11	7.891	2041	2053	2072	rBV	194135	342207	79.87%	9.240%
12	8.177	2132	2142	2160	rBV2	24823	44446	10.37%	1.200%
13	8.467	2222	2232	2245	rVB2	7887	13476	3.15%	0.364%
14	8.628	2272	2282	2314	rBV2	200384	412131	96.19%	11.128%
15	9.412	2514	2526	2551	rBV	235414	404691	94.45%	10.927%
16	10.750	2931	2942	2967	rBV	67635	113023	26.38%	3.052%
17	10.888	2973	2985	2997	rVB	22737	37217	8.69%	1.005%
18	11.807	3259	3271	3295	rBV	226701	374001	87.29%	10.098%
19	12.187	3378	3389	3413	rBV	173531	294738	68.79%	7.958%
20	12.766	3557	3569	3587	rBV	16504	26677	6.23%	0.720%
21	14.569	4121	4130	4142	rBV2	3696	6007	1.40%	0.162%




Sum of corrected areas: 3703589

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031324\
Data File : VU058077.D
Acq On : 13 Mar 2024 13:36
Operator : MD/SY
Sample : P1741-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

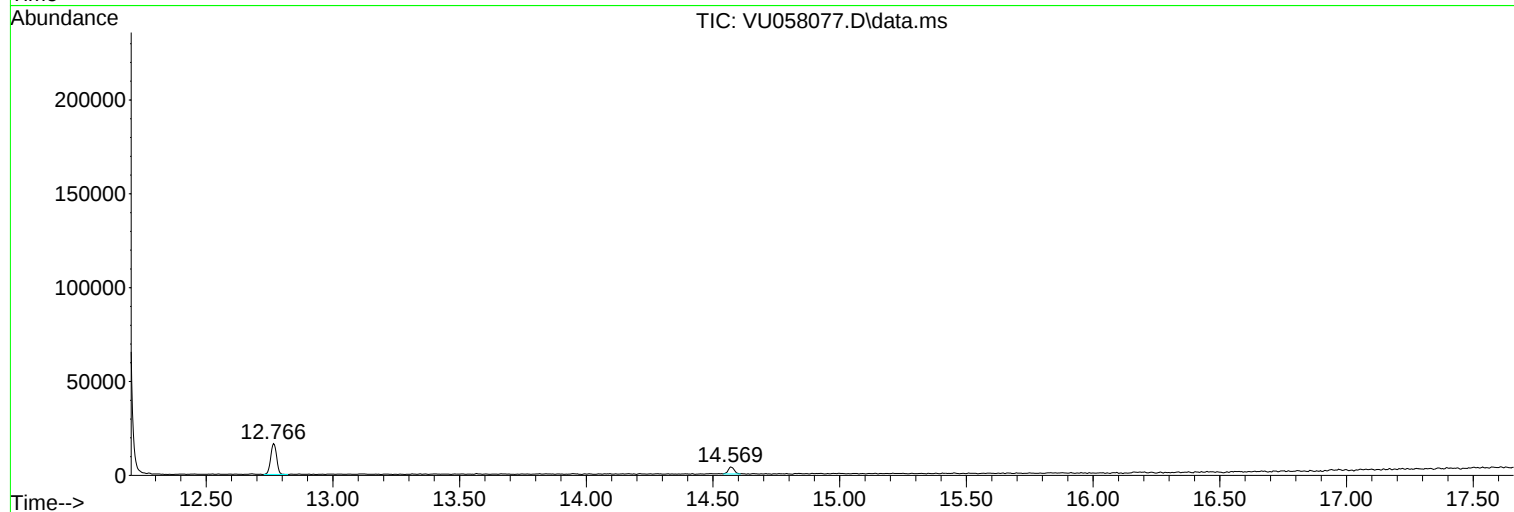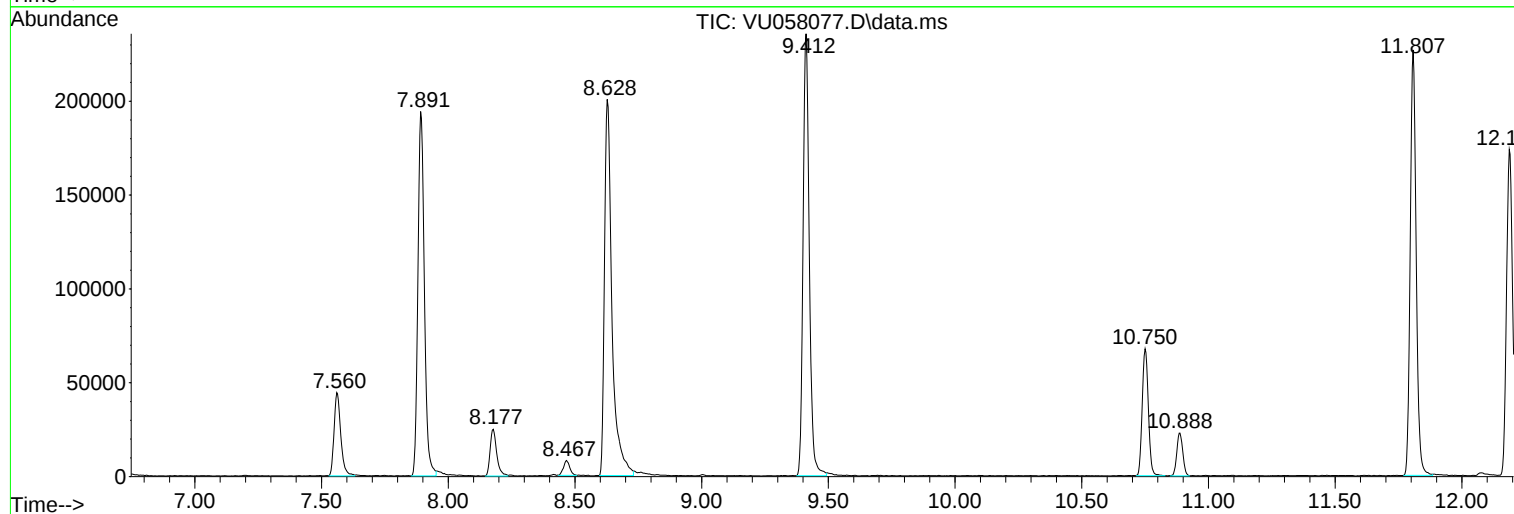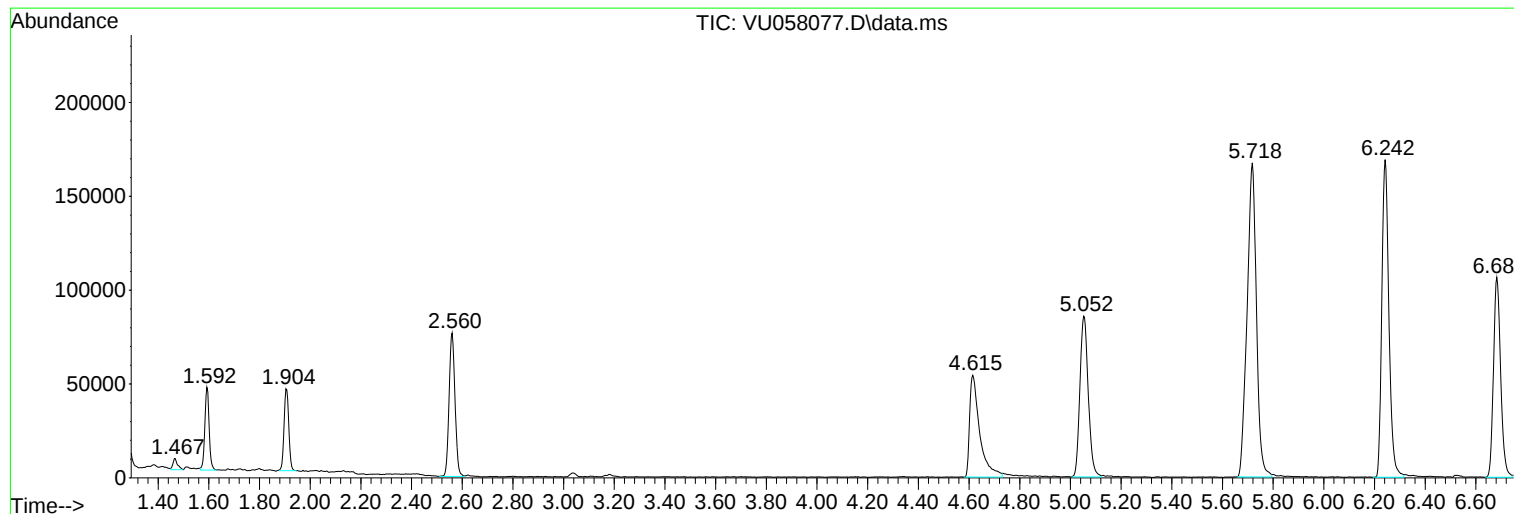

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031324\
Data File : VU058077.D
Acq On : 13 Mar 2024 13:36
Operator : MD/SY
Sample : P1741-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031324\
Data File : VU058077.D
Acq On : 13 Mar 2024 13:36
Operator : MD/SY
Sample : P1741-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc