

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031424\
 Data File : VU058097.D
 Acq On : 14 Mar 2024 13:08
 Operator : MD/SY
 Sample : P1729-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AJ9

Quant Time: Mar 15 01:20:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 14 04:37:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	129501	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	125162	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	56076	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	51281	5.504	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	110.000%
7) Chloroethane-d5	1.904	69	43719	5.709	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	114.200%
11) 1,1-Dichloroethene-d2	2.560	65	22878	5.674	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	113.400%
20) 2-Butanone-d5	4.615	46	84140	54.807	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.620%
24) Chloroform-d	5.052	84	93951	5.331	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.600%
26) 1,2-Dichloroethane-d4	5.695	65	44370	5.557	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.200%
32) Benzene-d6	5.718	84	192985	5.291	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.800%
36) 1,2-Dichloropropane-d6	6.682	67	59812	5.394	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.800%
41) Toluene-d8	7.891	98	164484	4.977	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.600%
43) trans-1,3-Dichloroprop...	8.177	79	16956	4.447	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.000%
46) 2-Hexanone-d5	8.627	63	68779	53.724	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.440%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	35118	5.165	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.200%
66) 1,2-Dichlorobenzene-d4	12.187	152	50810	5.502	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.000%
Target Compounds						
					Qvalue	
13) Acetone	2.621	43	10461	9.156	ug/L	98
21) 2-Butanone	4.714	43	6163	3.423	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031424\
Data File : VU058097.D
Acq On : 14 Mar 2024 13:08
Operator : MD/SY
Sample : P1729-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AJ9

Quant Time: Mar 15 01:20:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 14 04:37:22 2024
Response via : Initial Calibration

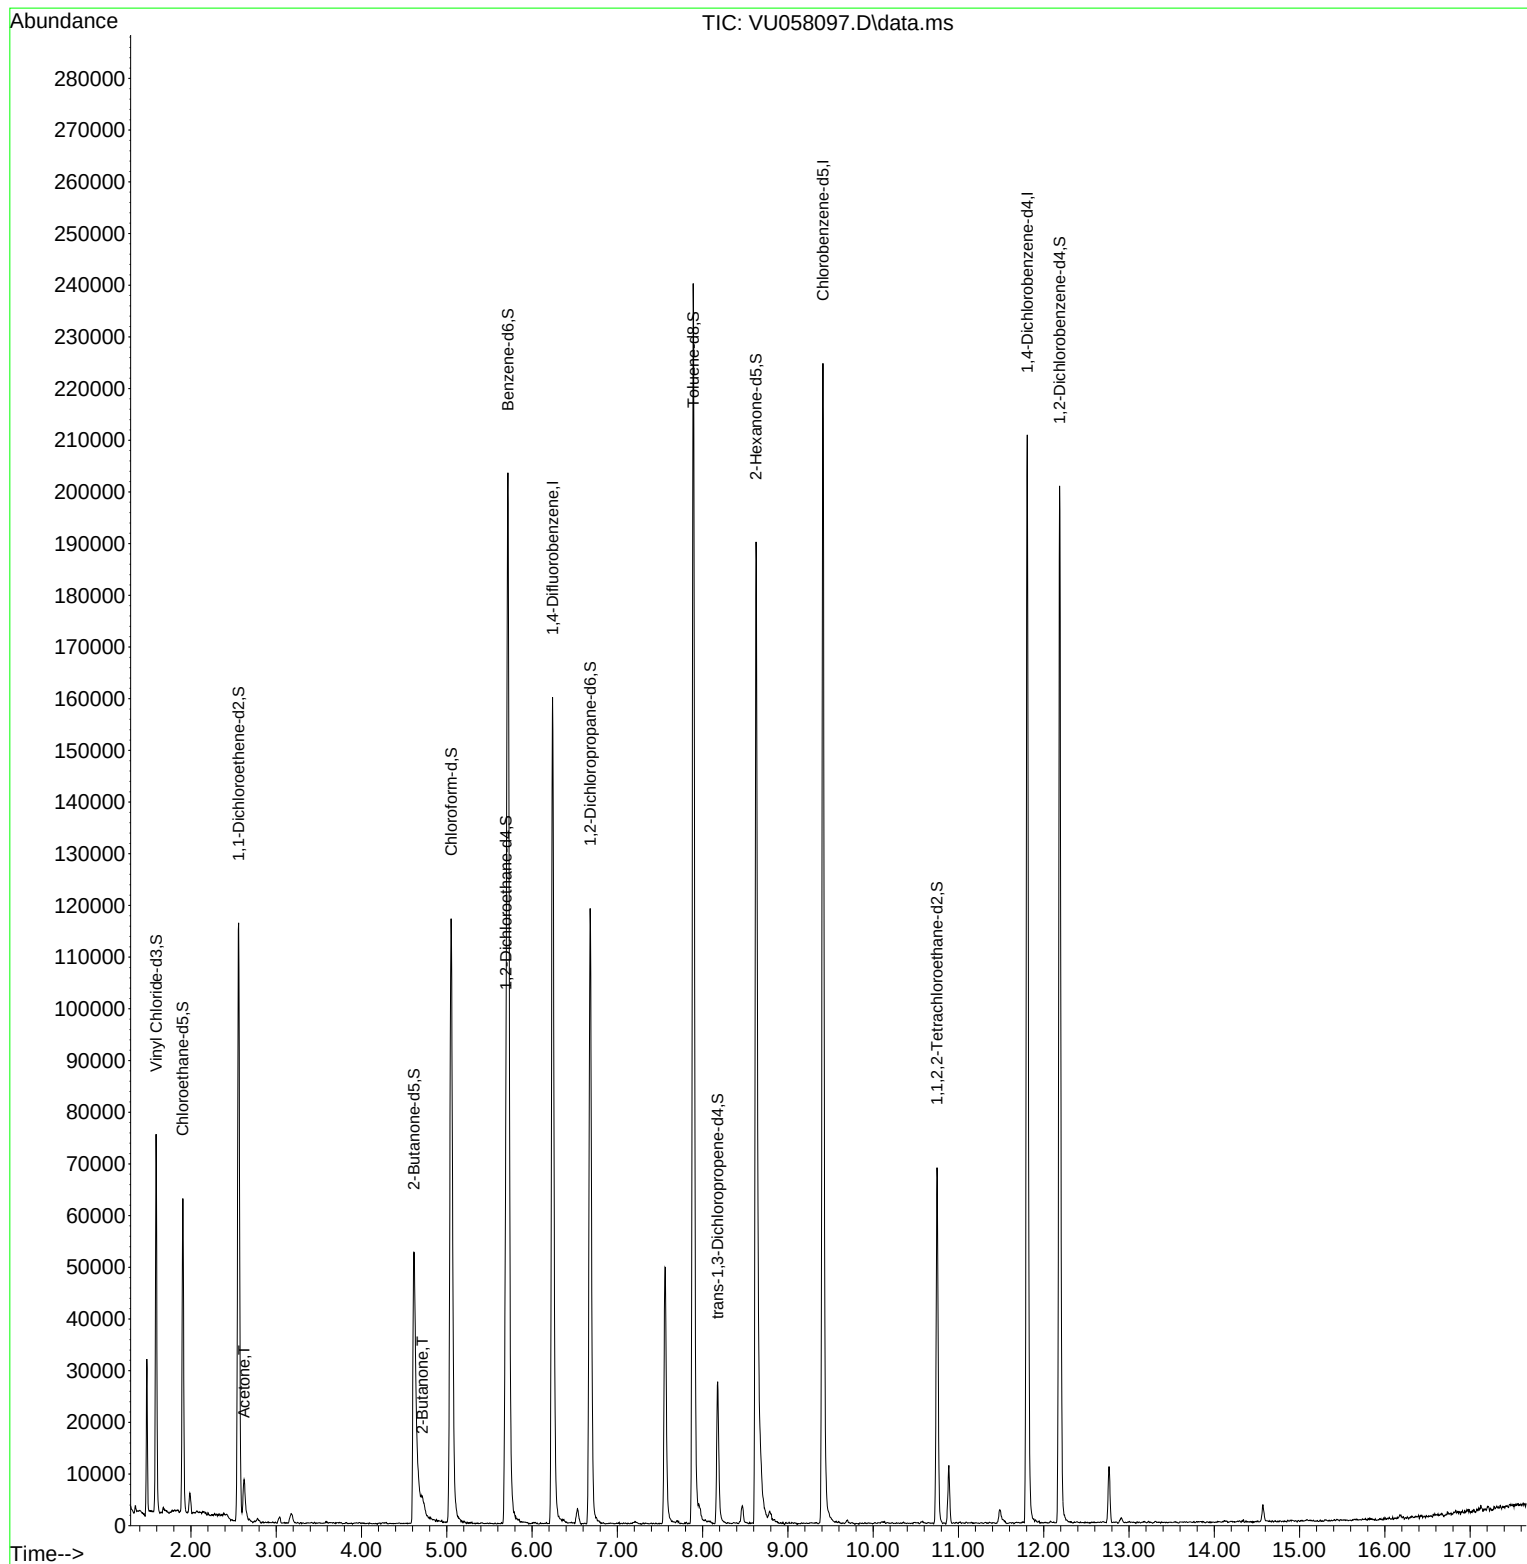

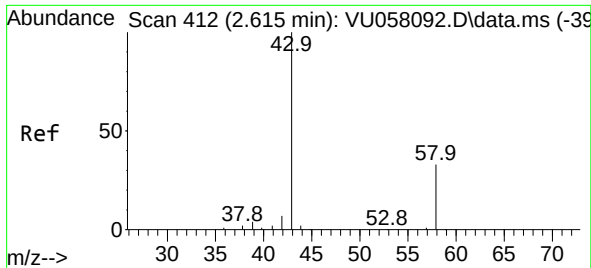

#13

Acetone

Concen: 9.156 ug/L

RT: 2.621 min Scan# 41

Delta R.T. -0.003 min

Lab File: VU058097.D

Acq: 14 Mar 2024 13:08

Instrument :

MSVOA_U

ClientSampleId :





C0AJ9

Tgt Ion: 43 Resp: 10461

Ion Ratio Lower Upper

43 100

58 30.9 0.0 63.6

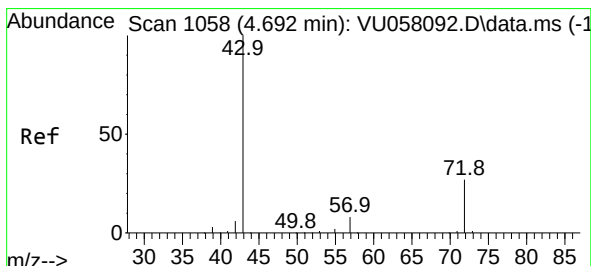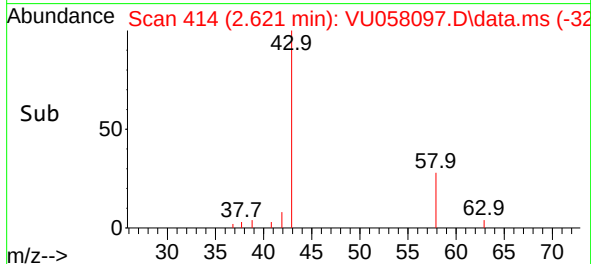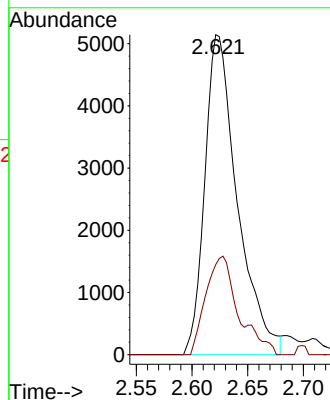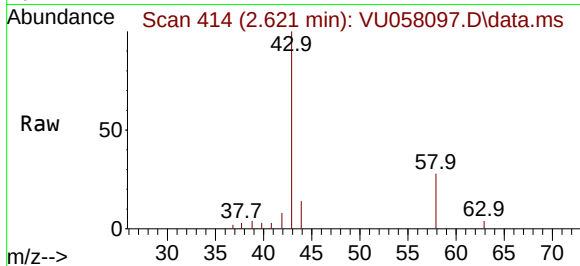

#21

2-Butanone

Concen: 3.423 ug/L

RT: 4.714 min Scan# 1065

Delta R.T. 0.016 min

Lab File: VU058097.D

Acq: 14 Mar 2024 13:08

Tgt Ion: 43 Resp: 6163

Ion Ratio Lower Upper

43 100

72 28.3 13.0 39.0

