

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031424\
 Data File : VU058107.D
 Acq On : 14 Mar 2024 17:21
 Operator : MD/SY
 Sample : P1741-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0GK2

Quant Time: Mar 15 01:21:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 14 04:37:22 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		6.242	114	127504	5.000	ug/L	0.00
28) Chlorobenzene-d5		9.412	117	124758	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.807	152	56041	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.592	65	54268	5.916	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	118.400%	
7) Chloroethane-d5		1.907	69	46089	6.113	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	122.200%	
11) 1,1-Dichloroethene-d2		2.560	65	24245	6.107	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	122.200%	
20) 2-Butanone-d5		4.611	46	89638	59.303	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.600%	
24) Chloroform-d		5.052	84	101662	5.859	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	117.200%	
26) 1,2-Dichloroethane-d4		5.692	65	48217	6.133	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	122.600%	
32) Benzene-d6		5.717	84	203091	5.586	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.800%	
36) 1,2-Dichloropropane-d6		6.682	67	64049	5.795	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	115.800%	
41) Toluene-d8		7.891	98	172419	5.234	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.600%	
43) trans-1,3-Dichloroprop...		8.177	79	18169	4.780	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.600%	
46) 2-Hexanone-d5		8.627	63	75309	59.015	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	118.040%	
56) 1,1,2,2-Tetrachloroeth...		10.749	84	39031	5.759	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	115.200%	
66) 1,2-Dichlorobenzene-d4		12.190	152	54428	5.897	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.000%	
Target Compounds							
13) Acetone		2.618	43	8876	7.891	ug/L	97
25) Chloroform		5.078	83	21075	1.235	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031424\
Data File : VU058107.D
Acq On : 14 Mar 2024 17:21
Operator : MD/SY
Sample : P1741-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GK2

Quant Time: Mar 15 01:21:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 14 04:37:22 2024
Response via : Initial Calibration

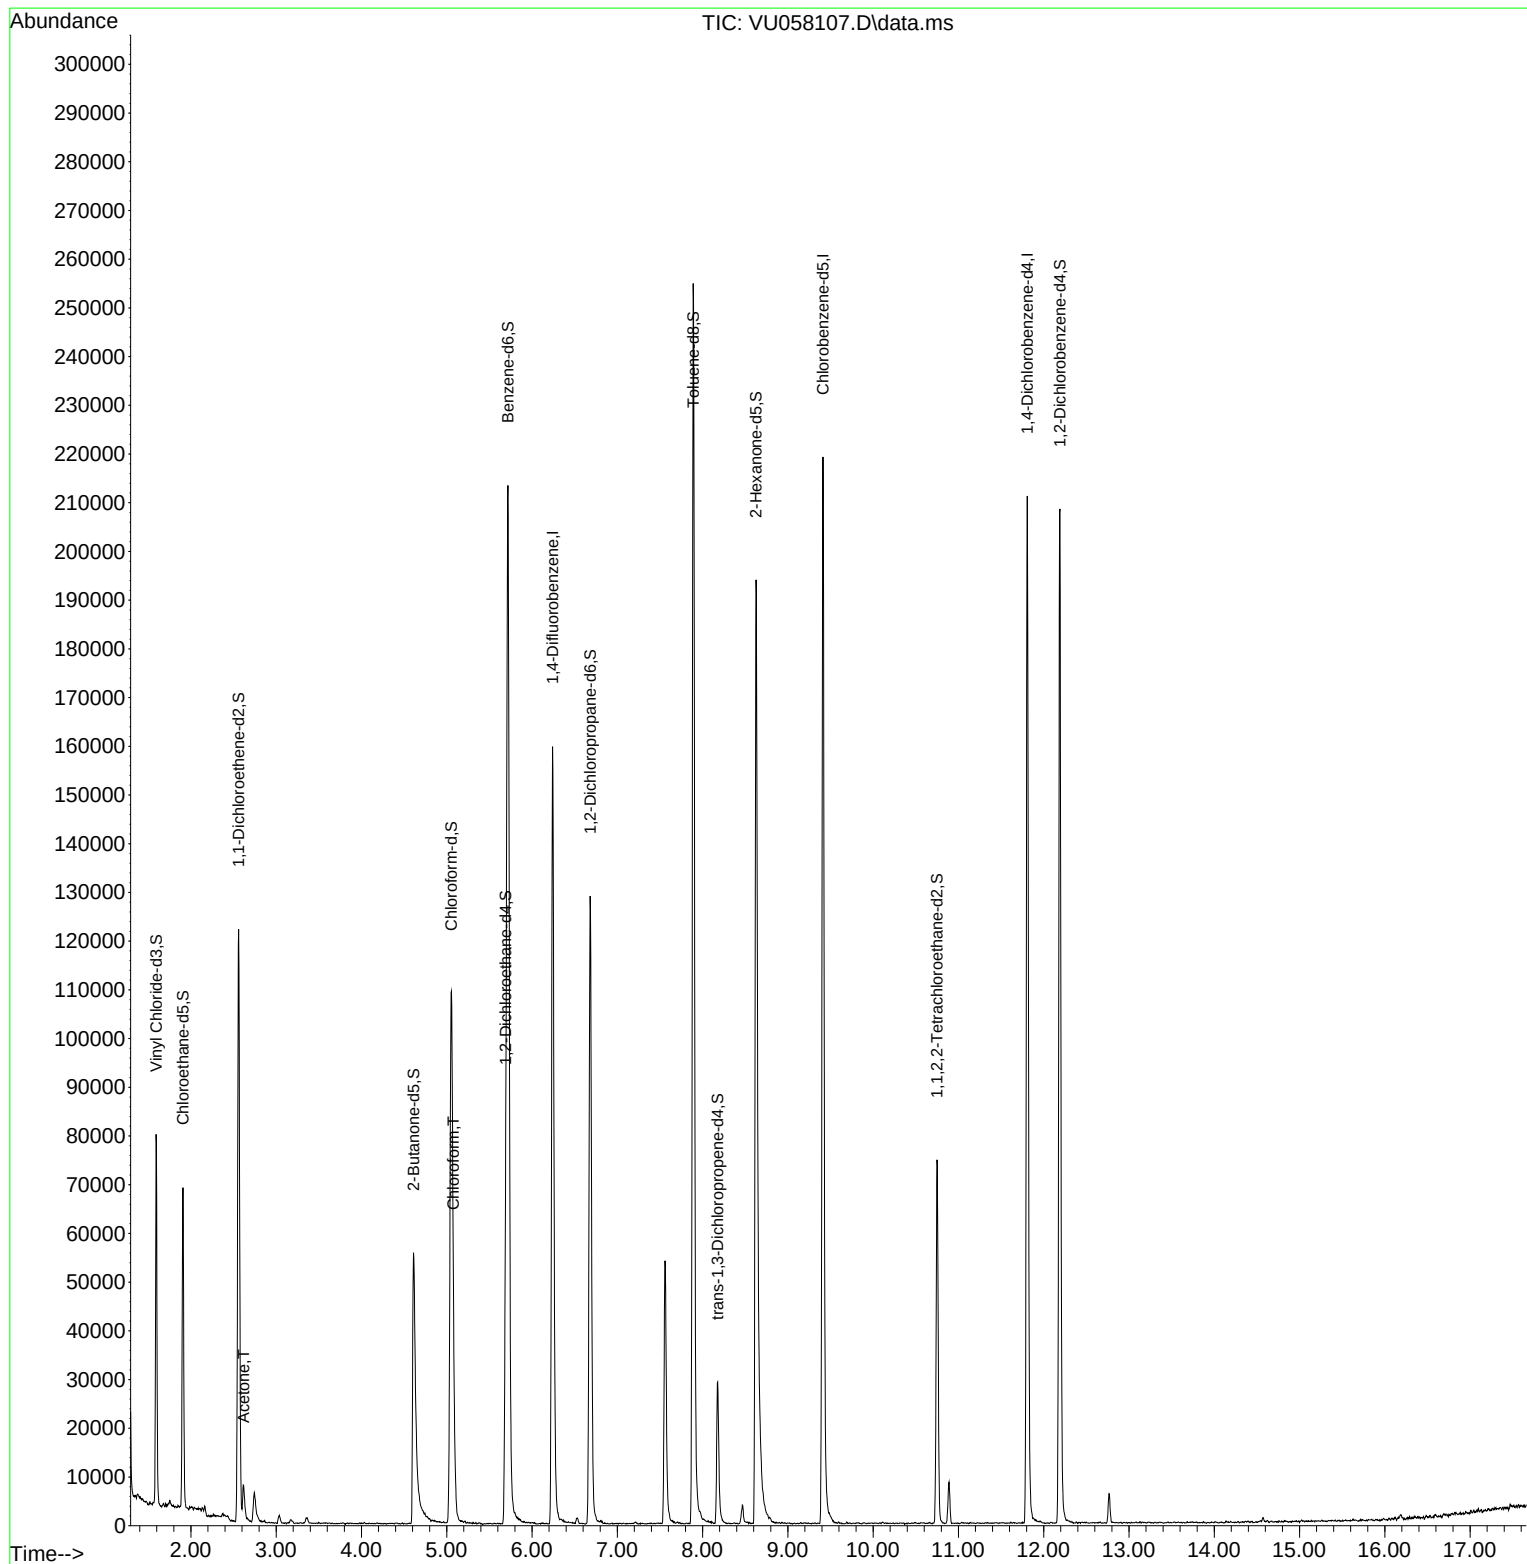

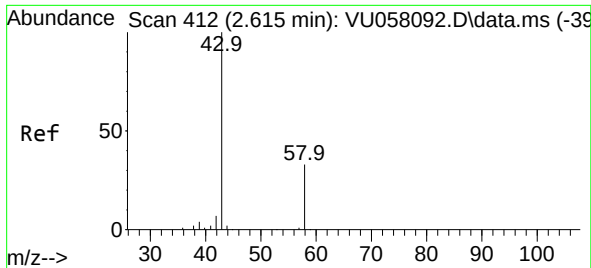

#13

Acetone

Concen: 7.891 ug/L

RT: 2.618 min Scan# 41

Delta R.T. -0.007 min

Lab File: VU058107.D

Acq: 14 Mar 2024 17:21

Instrument :

MSVOA_U

ClientSampleId :





C0GK2

Tgt Ion: 43 Resp: 8876

Ion Ratio Lower Upper

43 100

58 33.6 0.0 63.6

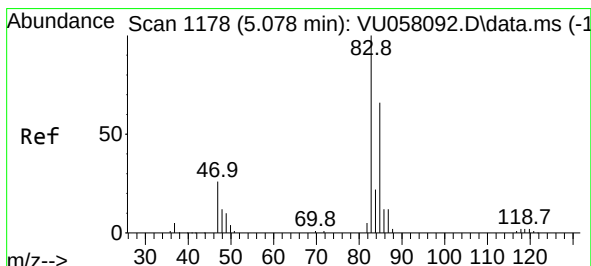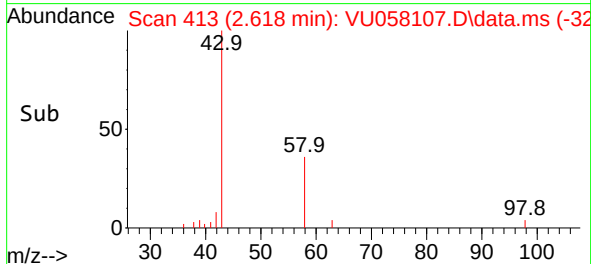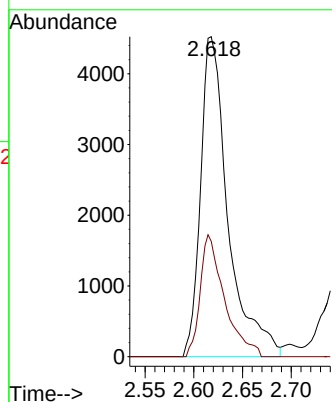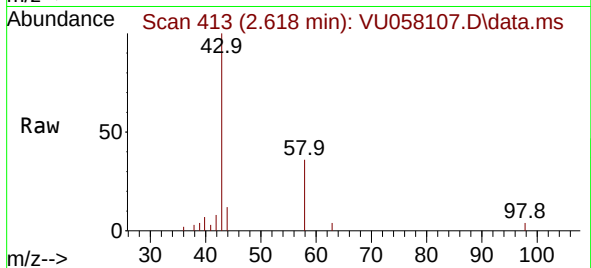

#25

Chloroform

Concen: 1.235 ug/L

RT: 5.078 min Scan# 1178

Delta R.T. -0.000 min

Lab File: VU058107.D

Acq: 14 Mar 2024 17:21

Tgt Ion: 83 Resp: 21075

Ion Ratio Lower Upper

83 100

85 61.8 45.4 84.4

