


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031424\
Data File : VU058091.D
Acq On : 14 Mar 2024 10:12
Operator : MD/SY
Sample : BFB122
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB122

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Mar 14 04:37:22 2024

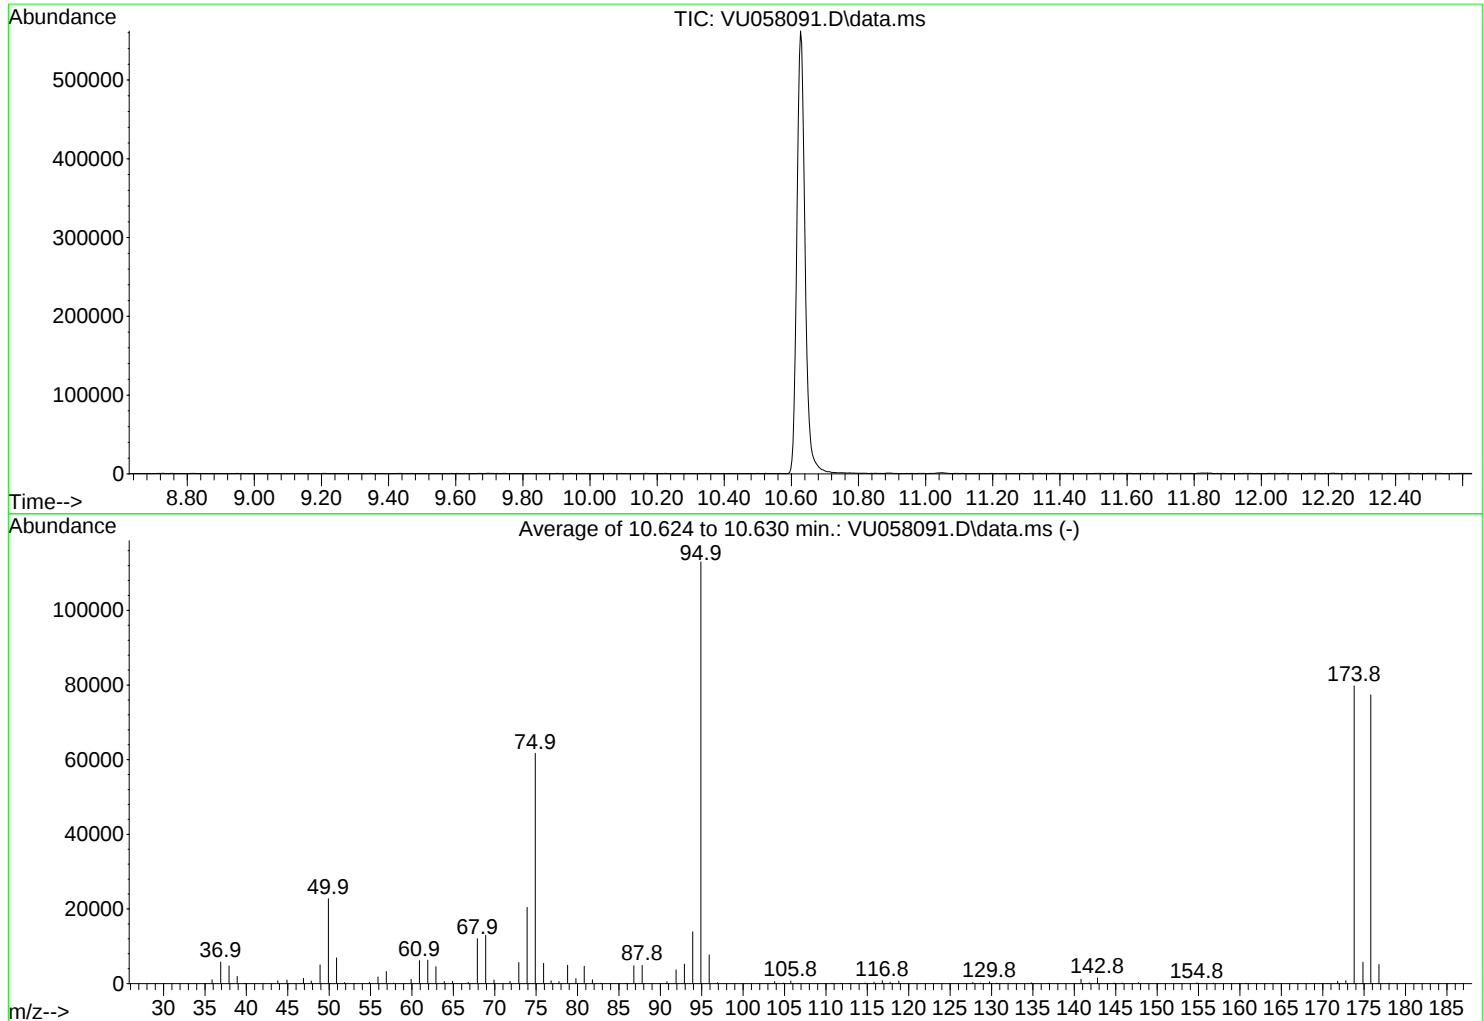

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.2	22771	PASS
75	95	30	80	54.6	61669	PASS
95	95	100	100	100.0	112992	PASS
96	95	5	9	6.8	7705	PASS
173	174	0.00	2	1.0	827	PASS
174	95	50	120	70.6	79781	PASS
175	174	5	9	7.2	5752	PASS
176	174	95	101	97.0	77349	PASS
177	176	5	9	6.7	5162	PASS

m/z	Abundance
39.90	118.0
43.80	276.0

Instrument :
MSVOA_U
ClientSampleId :
BFB122

m/z	Abundance
35.90	966.0
36.90	5635.0
37.90	4733.0
38.90	1814.0
39.80	241.0
43.90	1036.0
44.90	938.0
46.90	1470.0
47.90	692.0
48.90	4961.0
49.90	22032.0
50.90	6733.0
51.90	285.0
53.00	107.0
54.90	411.0
55.90	1789.0
56.90	3269.0
57.80	189.0
59.90	1177.0
60.90	5974.0
61.90	6257.0
62.90	4521.0
63.90	581.0
64.90	633.0
66.80	368.0
67.90	11819.0
68.90	12735.0
69.90	1064.0
71.80	582.0
72.90	5716.0
73.90	20344.0
74.90	60664.0
75.90	5337.0
76.80	759.0
77.70	603.0
78.80	4805.0
79.80	1227.0
80.80	4611.0
81.80	1013.0
82.80	142.0
85.80	140.0
86.80	4734.0
87.80	4794.0
90.80	530.0
91.90	3564.0
92.90	5038.0
93.90	13547.0
94.90	109712.0
95.90	7585.0
96.90	259.0
103.80	563.0
104.90	174.0
105.70	671.0
110.80	117.0
111.80	171.0
114.70	166.0
115.80	405.0
116.80	893.0
117.70	403.0
118.80	697.0
127.80	341.0
128.70	145.0
129.80	441.0
130.70	176.0
134.80	230.0
136.90	144.0
140.80	1176.0
141.80	192.0
142.80	1445.0
144.80	155.0
145.80	174.0
147.80	240.0
152.80	112.0
154.80	203.0
156.80	203.0
160.80	140.0
171.80	600.0
172.80	724.0
173.80	75200.0
174.90	5603.0
175.80	73216.0
176.80	5097.0
178.00	176.0

Instrument :
MSVOA_U
ClientSampleId :
BFB122

m/z	Abundance
35.80	1060.0
36.90	5969.0
37.90	4898.0
38.90	1982.0
39.80	215.0
43.90	1067.0
44.90	1002.0
46.90	1462.0
47.90	739.0
48.90	5110.0
49.90	23504.0
50.90	7058.0
51.80	286.0
54.90	427.0
55.90	1834.0
56.90	3355.0
57.80	211.0
59.90	1208.0
60.90	6388.0
61.90	6489.0
62.90	4687.0
63.90	588.0
64.90	642.0
66.80	347.0
67.90	12404.0
68.90	13298.0
69.90	1020.0
71.90	654.0
72.90	5813.0
73.90	21016.0
74.90	63680.0
75.90	5616.0
76.80	808.0
77.80	552.0
78.80	5074.0
79.80	1416.0
80.80	4783.0
81.80	1083.0
82.80	132.0
86.00	149.0
86.80	4995.0
87.80	5133.0
90.80	583.0
91.90	3824.0
92.90	5344.0
93.90	14270.0
94.90	116608.0
95.90	8014.0
96.90	264.0
103.80	596.0
104.90	177.0
105.80	746.0
106.70	104.0
110.70	138.0
111.80	150.0
112.80	123.0
114.70	205.0
115.80	440.0
116.80	809.0
117.80	369.0
118.80	765.0
127.70	367.0
128.60	161.0
129.80	485.0
130.60	188.0
134.80	256.0
136.80	138.0
140.80	1237.0
141.80	220.0
142.80	1595.0
144.80	149.0
145.70	152.0
147.70	266.0
154.80	217.0
156.80	190.0
160.80	123.0
171.80	653.0
172.80	849.0
173.80	82280.0
174.90	5897.0
175.80	79648.0
176.80	5288.0
178.00	159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB122

m/z	Abundance
35.80	1012.0
36.90	5699.0
37.90	4697.0
38.90	1989.0
39.80	174.0
43.80	1106.0
44.90	1008.0
46.90	1384.0
47.80	738.0
48.90	4932.0
49.90	22776.0
50.90	6924.0
51.80	269.0
54.80	378.0
55.90	1752.0
56.90	3225.0
57.80	182.0
59.90	1141.0
60.90	6133.0
61.90	6145.0
62.90	4476.0
63.90	515.0
64.90	621.0
66.80	304.0
67.90	11923.0
68.90	12756.0
69.90	867.0
71.90	657.0
72.90	5393.0
73.90	19952.0
74.90	60664.0
75.90	5325.0
76.80	778.0
77.80	508.0
78.80	4860.0
79.80	1412.0
80.80	4599.0
81.80	1025.0
82.80	113.0
85.70	111.0
86.00	117.0
86.80	4738.0
87.80	4753.0
90.80	573.0
91.90	3671.0
92.90	5268.0
93.90	13809.0
94.90	112656.0
95.90	7516.0
96.90	218.0
103.80	577.0
104.90	165.0
105.80	737.0
106.70	131.0
110.80	144.0
111.80	105.0
112.80	143.0
114.80	202.0
115.80	455.0
116.80	706.0
117.80	340.0
118.80	710.0
127.70	382.0
128.60	168.0
129.70	473.0
130.60	172.0
134.80	241.0
136.80	133.0
140.80	1252.0
141.80	189.0
142.80	1620.0
144.80	184.0
145.70	134.0
147.70	295.0
154.80	197.0
156.80	166.0
160.70	128.0
170.60	114.0
171.80	684.0
172.80	908.0
173.80	81864.0
174.80	5756.0
175.80	79184.0
176.80	5101.0
177.90	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB122