

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031522\
 Data File : VU047572.D
 Acq On : 15 Mar 2022 13:10
 Operator : SY/MD
 Sample : N1909-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Mar 16 06:45:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 16 06:43:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	134879	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	133707	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.813	152	67968	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	34705	3.934	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.600%
7) Chloroethane-d5	1.919	69	34681	4.332	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.600%
11) 1,1-Dichloroethene-d2	2.572	65	15326	3.705	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.000%
20) 2-Butanone-d5	4.646	46	145022	57.138	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.280%
24) Chloroform-d	5.067	84	86056	4.443	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.800%
26) 1,2-Dichloroethane-d4	5.703	65	49121	4.680	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.600%
32) Benzene-d6	5.732	84	162599	4.178	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.600%
36) 1,2-Dichloropropane-d6	6.694	67	55054	4.498	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.000%
41) Toluene-d8	7.900	98	136557	3.742	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.800%
43) trans-1,3-Dichloroprop...	8.182	79	21344	4.148	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.000%
46) 2-Hexanone-d5	8.636	63	125937	47.211	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.420%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	54826	4.485	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.800%
66) 1,2-Dichlorobenzene-d4	12.195	152	64004	4.506	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.200%
Target Compounds						Qvalue
3) Chloromethane	1.524	50	1670	0.205	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031522\
Data File : VU047572.D
Acq On : 15 Mar 2022 13:10
Operator : SY/MD
Sample : N1909-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001


Quant Time: Mar 16 06:45:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 16 06:43:54 2022
Response via : Initial Calibration

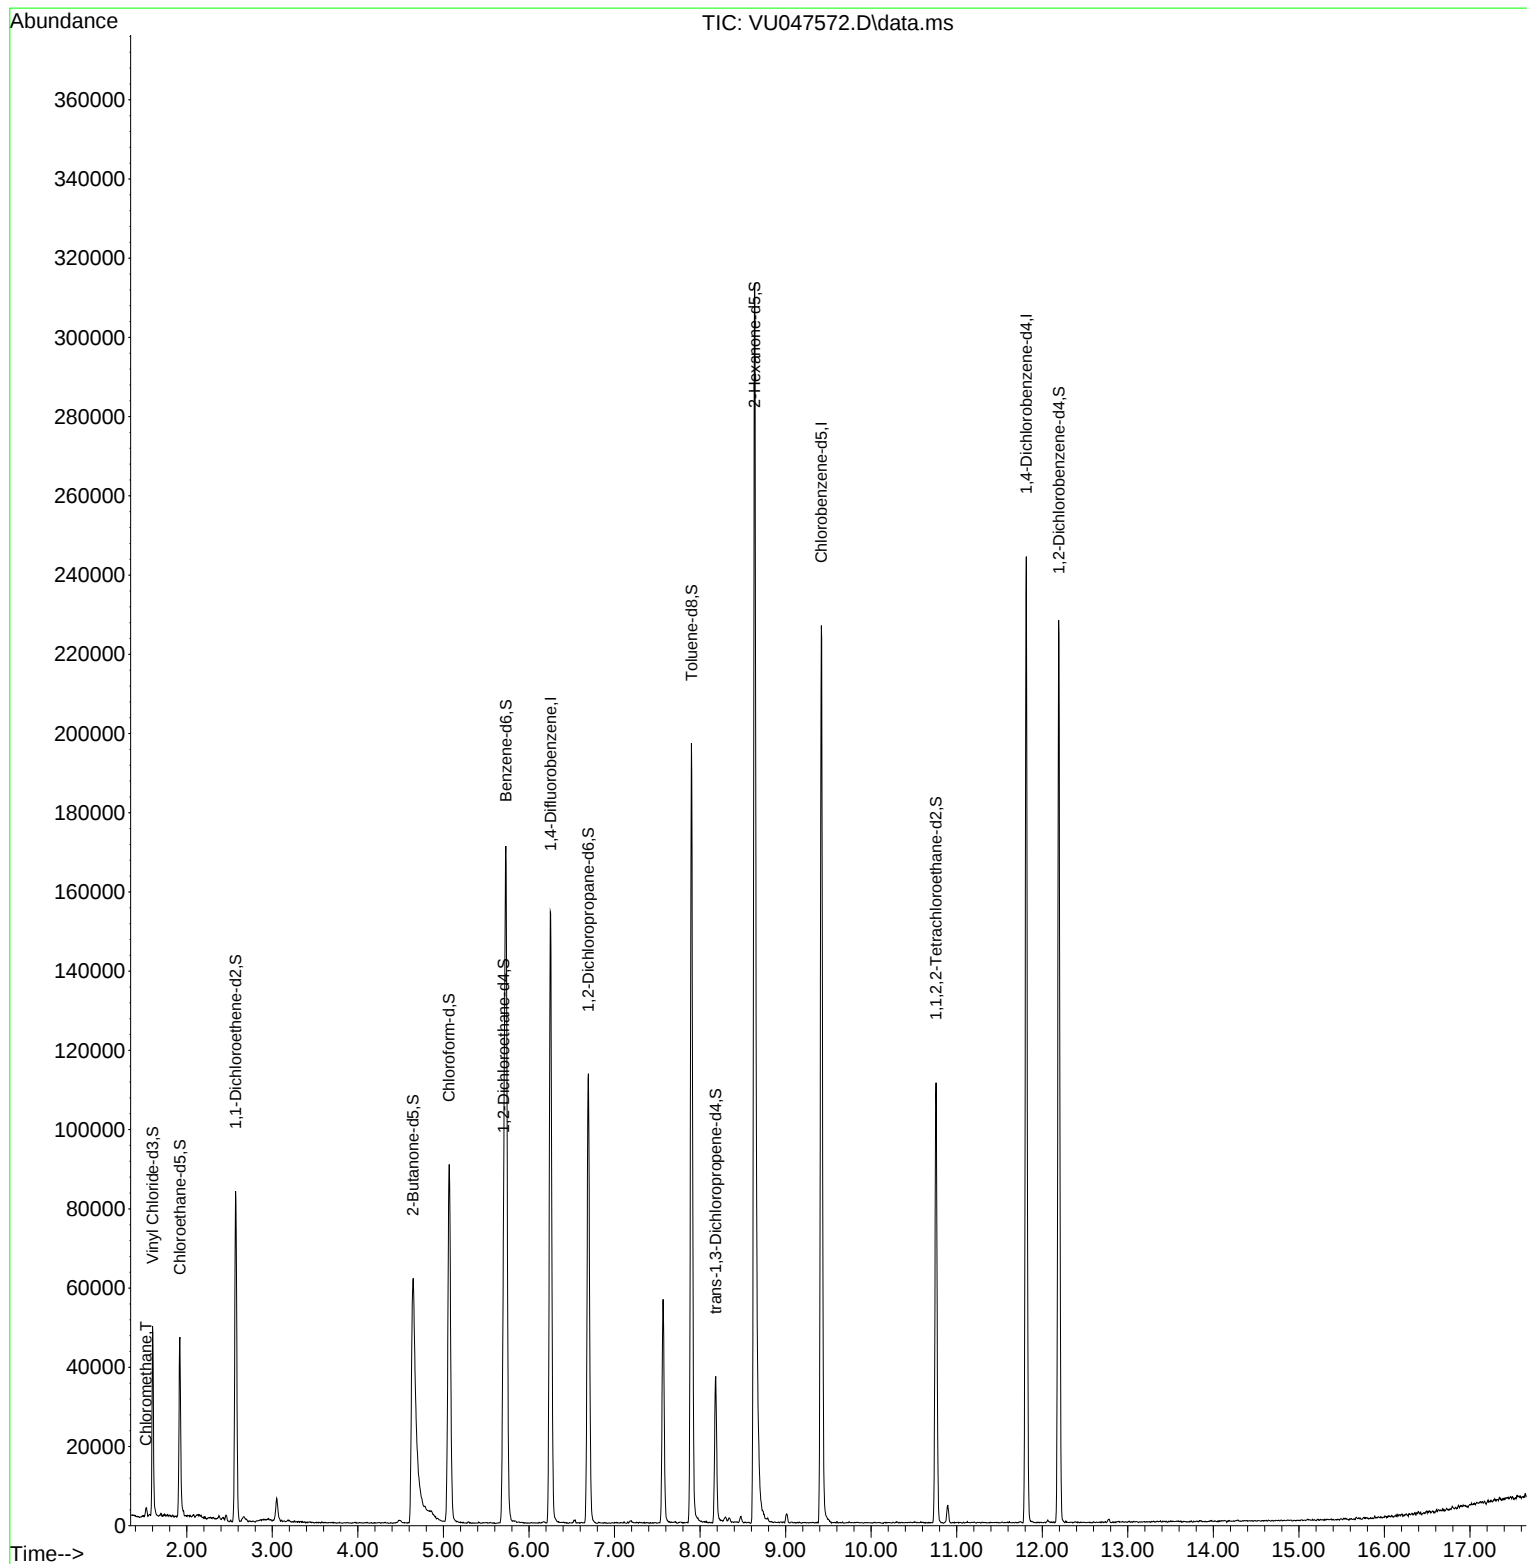

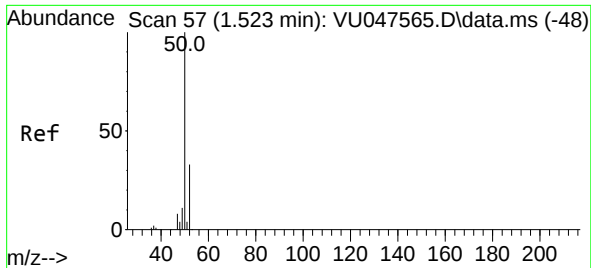

#3
 Chloromethane
 Concen: 0.205 ug/L
 RT: 1.524 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: VU047572.D
 Acq: 15 Mar 2022 13:10

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

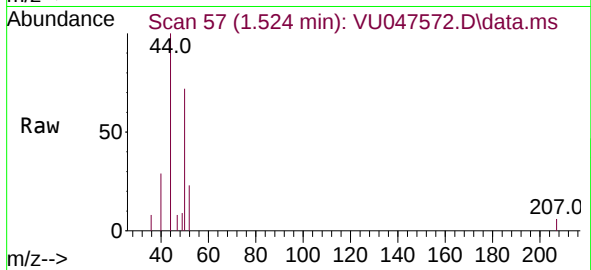

Tgt Ion: 50 Resp: 1670
 Ion Ratio Lower Upper
 50 100
 52 31.9 23.2 43.0

