

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031522\
 Data File : VU047575.D
 Acq On : 15 Mar 2022 14:21
 Operator : SY/MD
 Sample : N1858-22DL 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNK8DL

Quant Time: Mar 16 06:46:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 16 06:43:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	125670	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	124547	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	60844	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	32187	3.916	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.400%
7) Chloroethane-d5	1.919	69	33596	4.504	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.000%
11) 1,1-Dichloroethene-d2	2.572	65	14126	3.665	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.400%
20) 2-Butanone-d5	4.642	46	132768	56.144	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.280%
24) Chloroform-d	5.067	84	81612	4.522	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%
26) 1,2-Dichloroethane-d4	5.706	65	46942	4.800	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.000%
32) Benzene-d6	5.732	84	152201	4.198	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.000%
36) 1,2-Dichloropropane-d6	6.694	67	52044	4.565	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.200%
41) Toluene-d8	7.899	98	126610	3.724	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.400%
43) trans-1,3-Dichloroprop...	8.182	79	19973	4.167	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.400%
46) 2-Hexanone-d5	8.639	63	121243	48.794	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.580%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	53457	4.695	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.800%
66) 1,2-Dichlorobenzene-d4	12.195	152	59797	4.703	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.000%
Target Compounds						Qvalue
5) Vinyl chloride	1.607	62	43177	5.521	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031522\
Data File : VU047575.D
Acq On : 15 Mar 2022 14:21
Operator : SY/MD
Sample : N1858-22DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNK8DL

Quant Time: Mar 16 06:46:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 16 06:43:54 2022
Response via : Initial Calibration

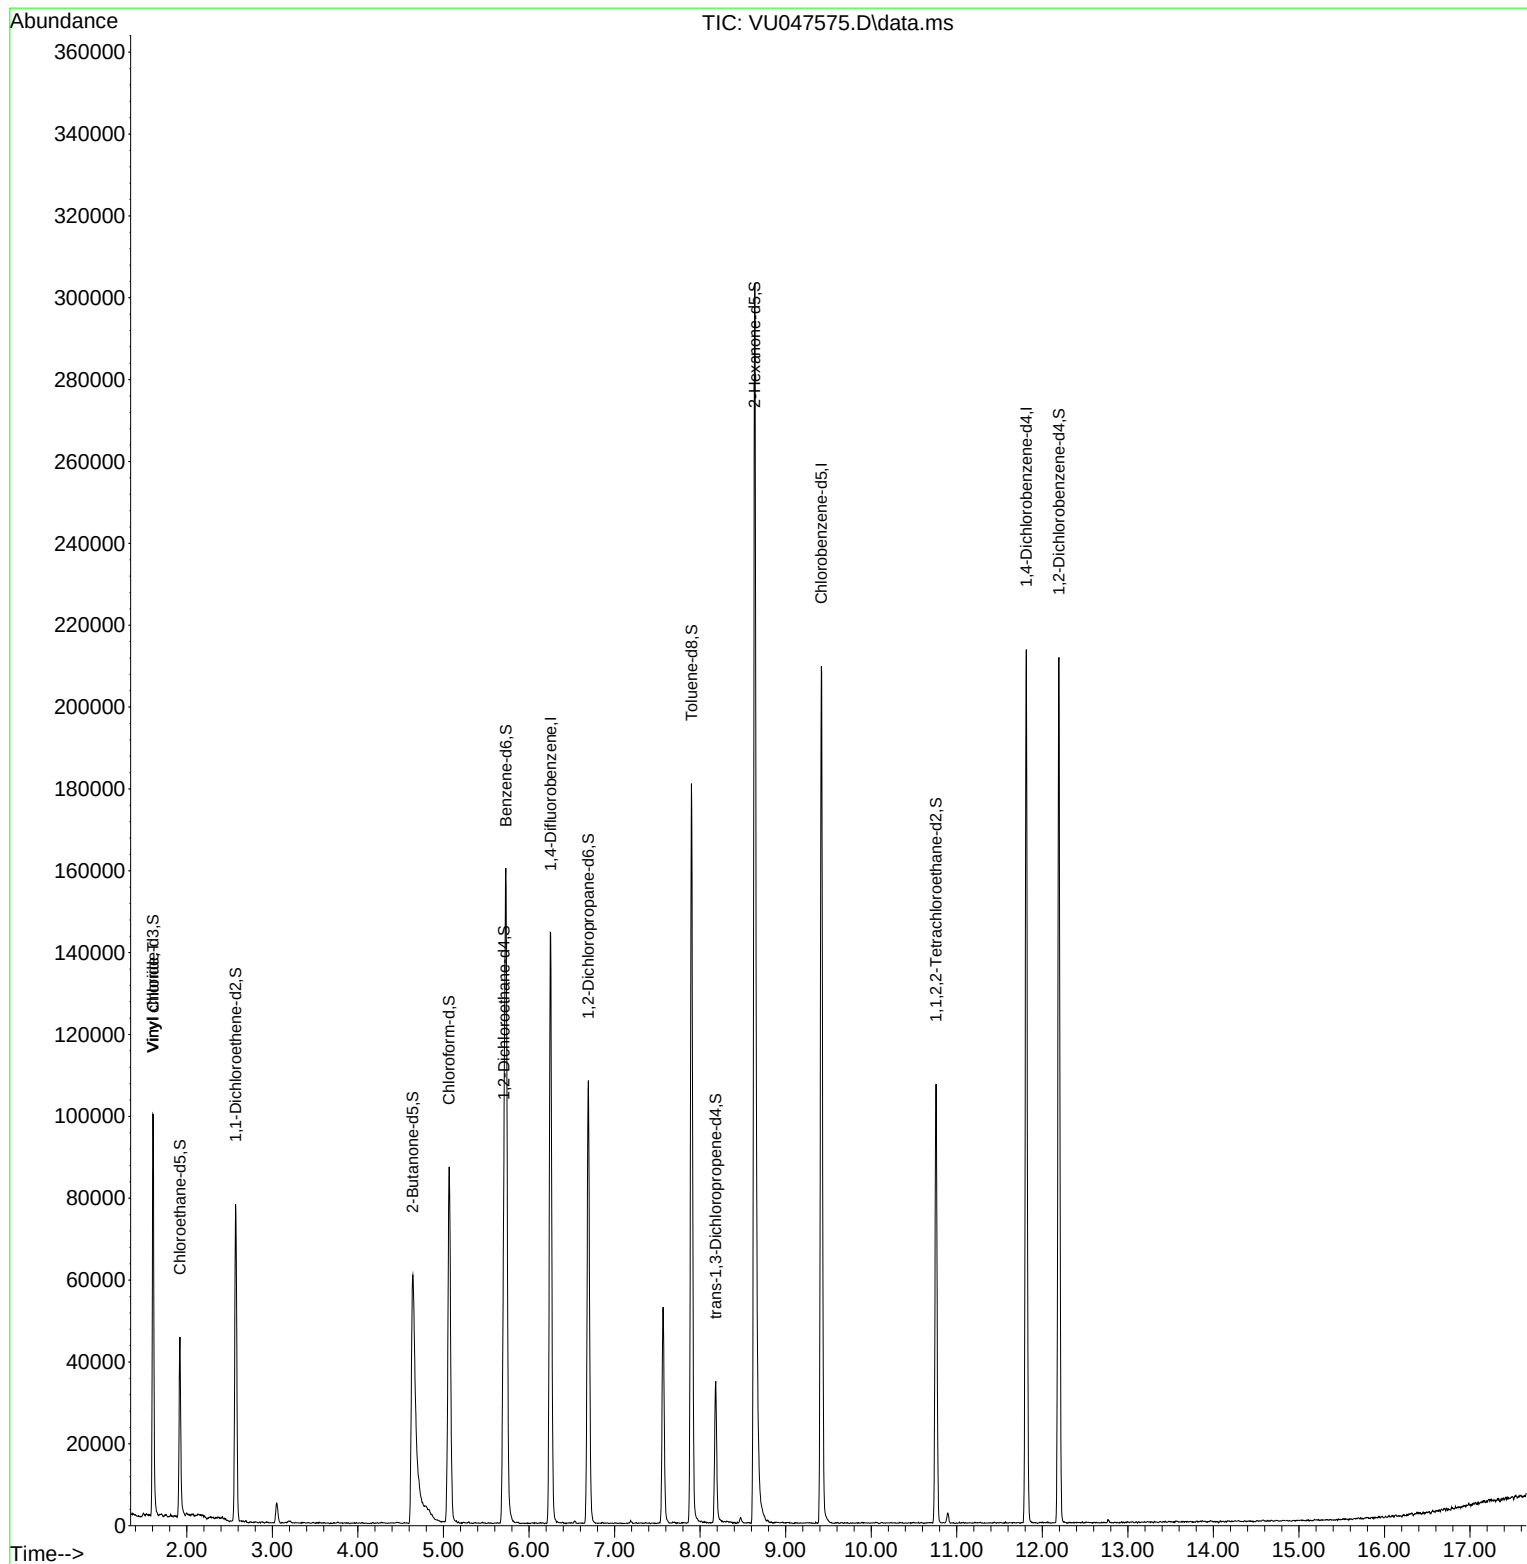

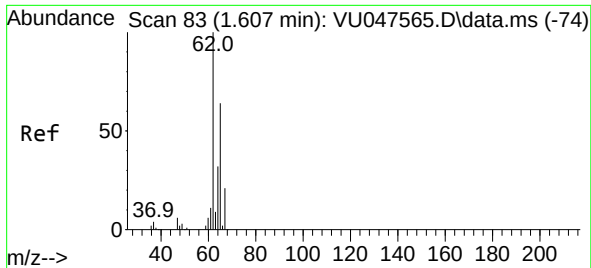

#5
 Vinyl chloride
 Concen: 5.521 ug/L
 RT: 1.607 min Scan# 81
 Delta R.T. -0.000 min
 Lab File: VU047575.D
 Acq: 15 Mar 2022 14:21

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNK8DL

Tgt Ion: 62 Resp: 43177
 Ion Ratio Lower Upper
 62 100
 64 32.4 23.5 43.7

