

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031522\
 Data File : VU047568.D
 Acq On : 15 Mar 2022 11:36
 Operator : SY/MD
 Sample : N1840-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU047568.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	73	82	96	rVB	47739	57519	9.22%	1.390%
2	1.919	170	180	197	rBV	46236	64498	10.34%	1.559%
3	2.575	369	384	396	rBV	84709	137527	22.05%	3.325%
4	3.054	523	533	542	rBV2	4680	8349	1.34%	0.202%
5	4.649	1013	1029	1065	rBV2	61938	242995	38.96%	5.874%
6	5.067	1143	1159	1178	rBV	92035	200551	32.16%	4.848%
7	5.729	1343	1365	1391	rBV2	172725	455867	73.09%	11.020%
8	6.253	1512	1528	1544	rBV	149157	286653	45.96%	6.929%
9	6.694	1651	1665	1687	rBV	113935	221424	35.50%	5.353%
10	7.568	1925	1937	1955	rBV	56046	100450	16.11%	2.428%
11	7.899	2027	2040	2059	rBV	197276	344868	55.30%	8.337%
12	8.182	2117	2128	2147	rBV	36539	62163	9.97%	1.503%
13	8.639	2257	2270	2304	rBV	322584	623669	100.00%	15.076%
14	8.790	2309	2317	2330	rVB4	7511	13244	2.12%	0.320%
15	9.417	2499	2512	2544	rBV	214927	365545	58.61%	8.837%
16	10.758	2916	2929	2945	rBV	112175	180105	28.88%	4.354%
17	10.893	2960	2971	2982	rVB3	4638	7675	1.23%	0.186%
18	11.812	3241	3257	3282	rBV	232111	368579	59.10%	8.910%
19	12.192	3363	3375	3391	rBV	228995	368949	59.16%	8.919%
20	12.889	3582	3592	3600	rBV2	9407	12325	1.98%	0.298%
21	16.883	4826	4834	4844	rBV2	9175	13789	2.21%	0.333%




Sum of corrected areas: 4136744

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031522\
Data File : VU047568.D
Acq On : 15 Mar 2022 11:36
Operator : SY/MD
Sample : N1840-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

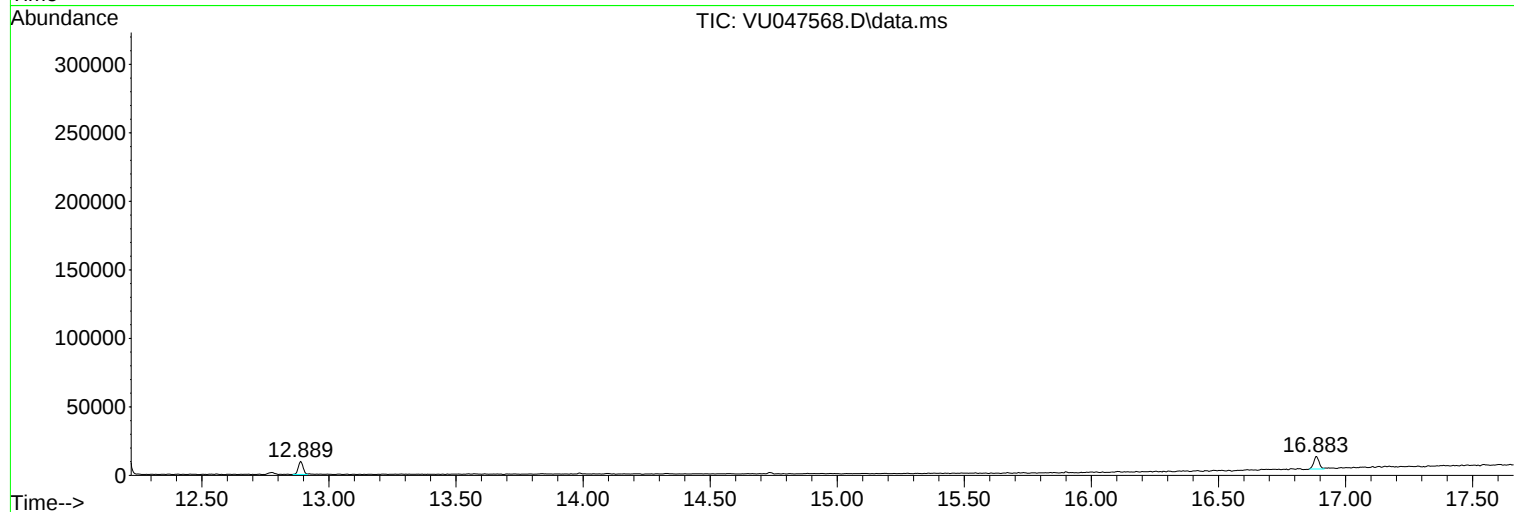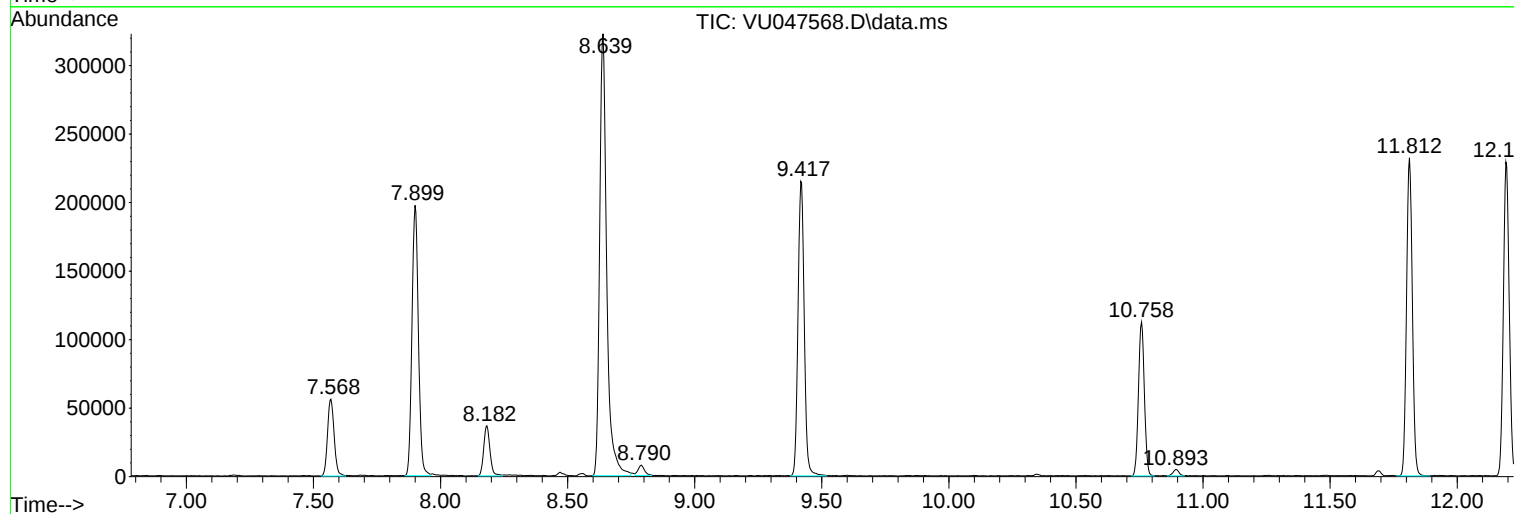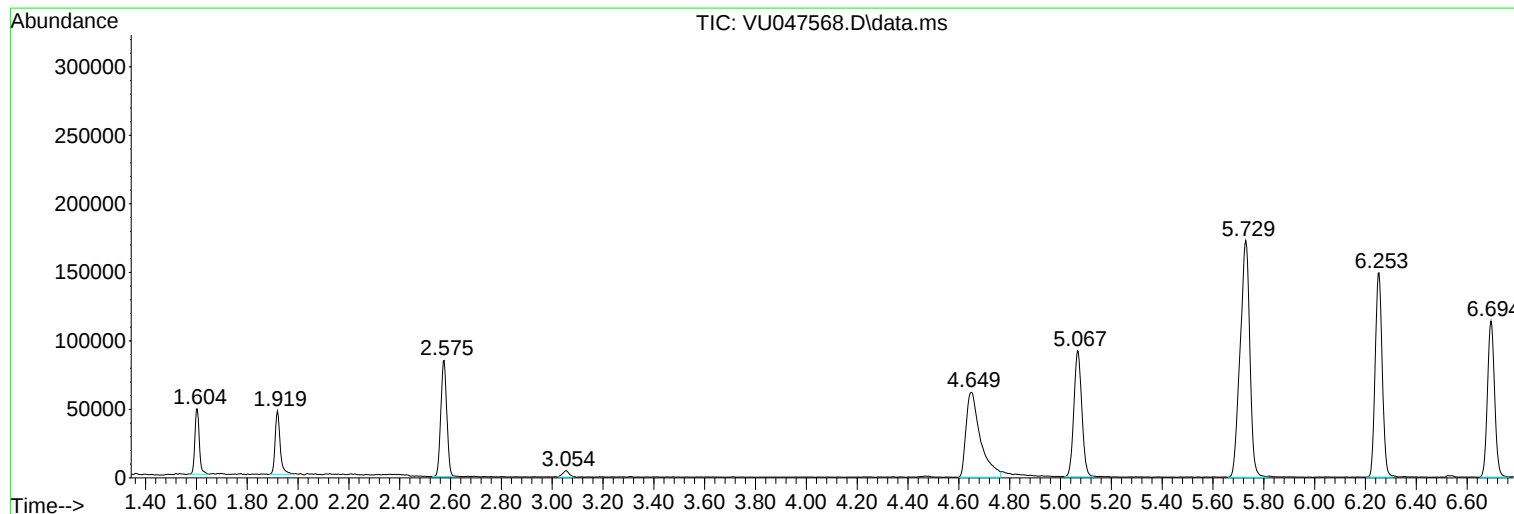

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031522\
Data File : VU047568.D
Acq On : 15 Mar 2022 11:36
Operator : SY/MD
Sample : N1840-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031522\
Data File : VU047568.D
Acq On : 15 Mar 2022 11:36
Operator : SY/MD
Sample : N1840-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc