


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031522\
 Data File : VU047564.D
 Acq On : 15 Mar 2022 09:00
 Operator : SY/MD
 Sample : BFB068
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB068

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Mar 18 01:27:05 2022

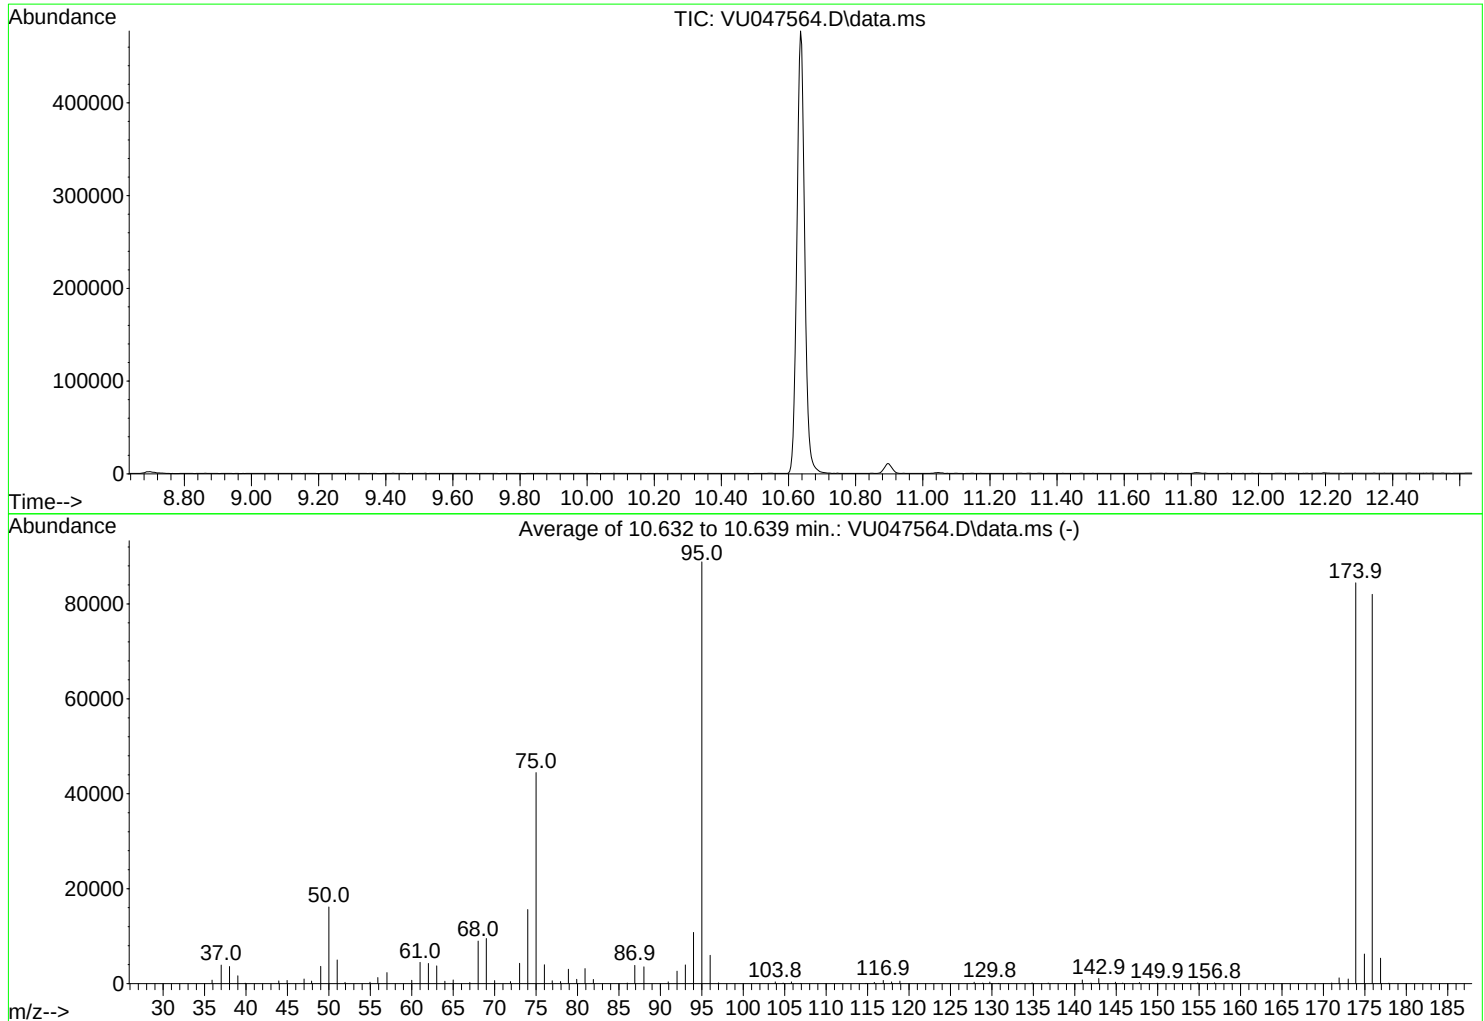

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	16159	PASS
75	95	30	80	50.0	44467	PASS
95	95	100	100	100.0	88864	PASS
96	95	5	9	6.7	5973	PASS
173	174	0.00	2	1.2	981	PASS
174	95	50	120	95.0	84432	PASS
175	174	5	9	7.4	6248	PASS
176	174	95	101	97.1	82019	PASS
177	176	5	9	6.5	5365	PASS

m/z	Abundance
39.90	238.0
43.90	254.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068

m/z	Abundance
35.90	787.0
37.00	3892.0
38.00	3792.0
39.00	1617.0
40.00	317.0
44.00	843.0
45.00	648.0
47.00	1040.0
47.90	521.0
49.00	3812.0
50.00	16109.0
51.00	5075.0
52.00	252.0
54.90	280.0
55.90	1203.0
57.00	2267.0
60.00	733.0
61.00	4306.0
62.00	4060.0
63.00	3751.0
64.00	499.0
65.00	775.0
67.00	245.0
68.00	8784.0
69.00	9248.0
70.00	632.0
71.90	405.0
73.00	4097.0
74.00	15015.0
75.00	43152.0
76.00	3997.0
76.90	479.0
78.00	374.0
78.90	3025.0
79.90	905.0
80.90	3064.0
81.90	843.0
86.00	152.0
86.90	3632.0
88.00	3464.0
90.90	371.0
92.00	2565.0
93.00	3910.0
94.00	10600.0
95.00	86488.0
96.00	5874.0
97.00	160.0
103.80	324.0
104.80	149.0
105.80	361.0
106.90	118.0
115.80	292.0
116.90	668.0
117.90	305.0
118.90	515.0
127.90	275.0
128.90	142.0
129.70	287.0
134.80	175.0
136.80	134.0
140.90	838.0
142.00	138.0
142.90	1001.0
144.90	297.0
145.80	131.0
147.80	252.0
149.90	107.0
154.90	149.0
156.90	175.0
171.00	139.0
171.90	1197.0
173.00	955.0
173.90	79704.0
174.90	6151.0
175.90	77608.0
176.90	5203.0
177.90	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068

m/z	Abundance
35.90	791.0
37.00	4037.0
38.00	3730.0
39.00	1748.0
39.90	320.0
44.00	854.0
45.00	699.0
47.00	1006.0
47.90	574.0
49.00	3735.0
50.00	16704.0
51.00	5130.0
51.90	284.0
54.90	306.0
55.90	1334.0
57.00	2378.0
60.00	740.0
61.00	4658.0
62.00	4360.0
63.00	3915.0
64.00	540.0
65.00	804.0
67.00	231.0
68.00	9252.0
69.00	9907.0
70.00	645.0
71.90	432.0
73.00	4462.0
74.00	16207.0
75.00	45872.0
76.00	4122.0
76.90	617.0
78.00	433.0
78.90	3079.0
79.90	924.0
80.90	3232.0
81.90	915.0
86.00	169.0
86.90	3972.0
88.00	3644.0
91.00	393.0
92.00	2732.0
93.00	4064.0
94.00	11071.0
95.00	91824.0
96.00	6207.0
97.00	176.0
103.80	370.0
104.80	146.0
105.80	385.0
106.90	110.0
114.80	120.0
115.80	282.0
116.90	727.0
117.90	373.0
118.90	560.0
127.80	284.0
128.90	150.0
129.80	335.0
130.80	116.0
134.90	180.0
136.80	122.0
140.90	802.0
142.00	139.0
142.90	1127.0
144.90	317.0
145.80	141.0
147.80	244.0
149.90	109.0
154.90	191.0
156.90	187.0
158.90	112.0
171.00	144.0
171.90	1251.0
173.00	1031.0
173.90	87368.0
174.90	6387.0
175.90	84680.0
176.90	5564.0
177.90	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068

m/z	Abundance
35.90	679.0
37.00	3834.0
38.00	3348.0
39.00	1631.0
39.90	351.0
44.00	746.0
44.90	678.0
47.00	871.0
47.90	554.0
49.00	3412.0
50.00	15664.0
51.00	4786.0
51.90	271.0
55.00	315.0
55.90	1288.0
57.00	2335.0
60.00	684.0
61.00	4467.0
62.00	4367.0
63.00	3606.0
64.00	518.0
65.00	788.0
67.00	218.0
68.00	8849.0
69.00	9351.0
70.00	628.0
71.90	451.0
73.00	4303.0
74.00	15621.0
75.00	44376.0
76.00	3834.0
77.00	698.0
77.90	465.0
78.90	2955.0
79.90	871.0
80.90	3238.0
81.90	860.0
86.00	134.0
86.90	3934.0
88.00	3566.0
90.90	343.0
92.00	2638.0
93.00	3900.0
94.00	10712.0
95.00	88280.0
96.00	5839.0
97.00	174.0
103.90	403.0
104.80	124.0
105.80	351.0
114.80	121.0
115.80	277.0
116.90	677.0
117.90	405.0
118.90	538.0
127.80	310.0
128.90	161.0
129.80	362.0
130.80	126.0
134.90	162.0
136.80	126.0
140.90	735.0
141.90	126.0
142.90	1136.0
144.90	284.0
145.80	131.0
147.80	211.0
150.00	109.0
154.80	210.0
156.80	194.0
158.90	107.0
171.00	123.0
171.90	1208.0
173.00	956.0
173.90	86224.0
175.00	6205.0
175.90	83768.0
176.90	5328.0
177.90	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068