

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031524\
 Data File : VU058130.D
 Acq On : 15 Mar 2024 16:20
 Operator : MD/SY
 Sample : P1777-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0GP6

Quant Time: Mar 15 23:31:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 14 04:37:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	127294	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	124156	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	52818	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	44673	4.878	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.600%
7) Chloroethane-d5	1.904	69	40424	5.370	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.400%
11) 1,1-Dichloroethene-d2	2.557	65	20382	5.143	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	102.800%
20) 2-Butanone-d5	4.612	46	83280	55.188	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.380%
24) Chloroform-d	5.052	84	87828	5.070	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.400%
26) 1,2-Dichloroethane-d4	5.695	65	42525	5.418	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.400%
32) Benzene-d6	5.718	84	177558	4.907	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
36) 1,2-Dichloropropane-d6	6.682	67	56862	5.170	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.400%
41) Toluene-d8	7.891	98	153548	4.684	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.600%
43) trans-1,3-Dichloroprop...	8.177	79	15159	4.008	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.200%
46) 2-Hexanone-d5	8.627	63	67027	52.780	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.560%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	34623	5.133	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.600%
66) 1,2-Dichlorobenzene-d4	12.190	152	45250	5.202	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.000%
Target Compounds						Qvalue
25) Chloroform	5.078	83	4544	0.267	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031524\
Data File : VU058130.D
Acq On : 15 Mar 2024 16:20
Operator : MD/SY
Sample : P1777-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GP6

Quant Time: Mar 15 23:31:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 14 04:37:22 2024
Response via : Initial Calibration

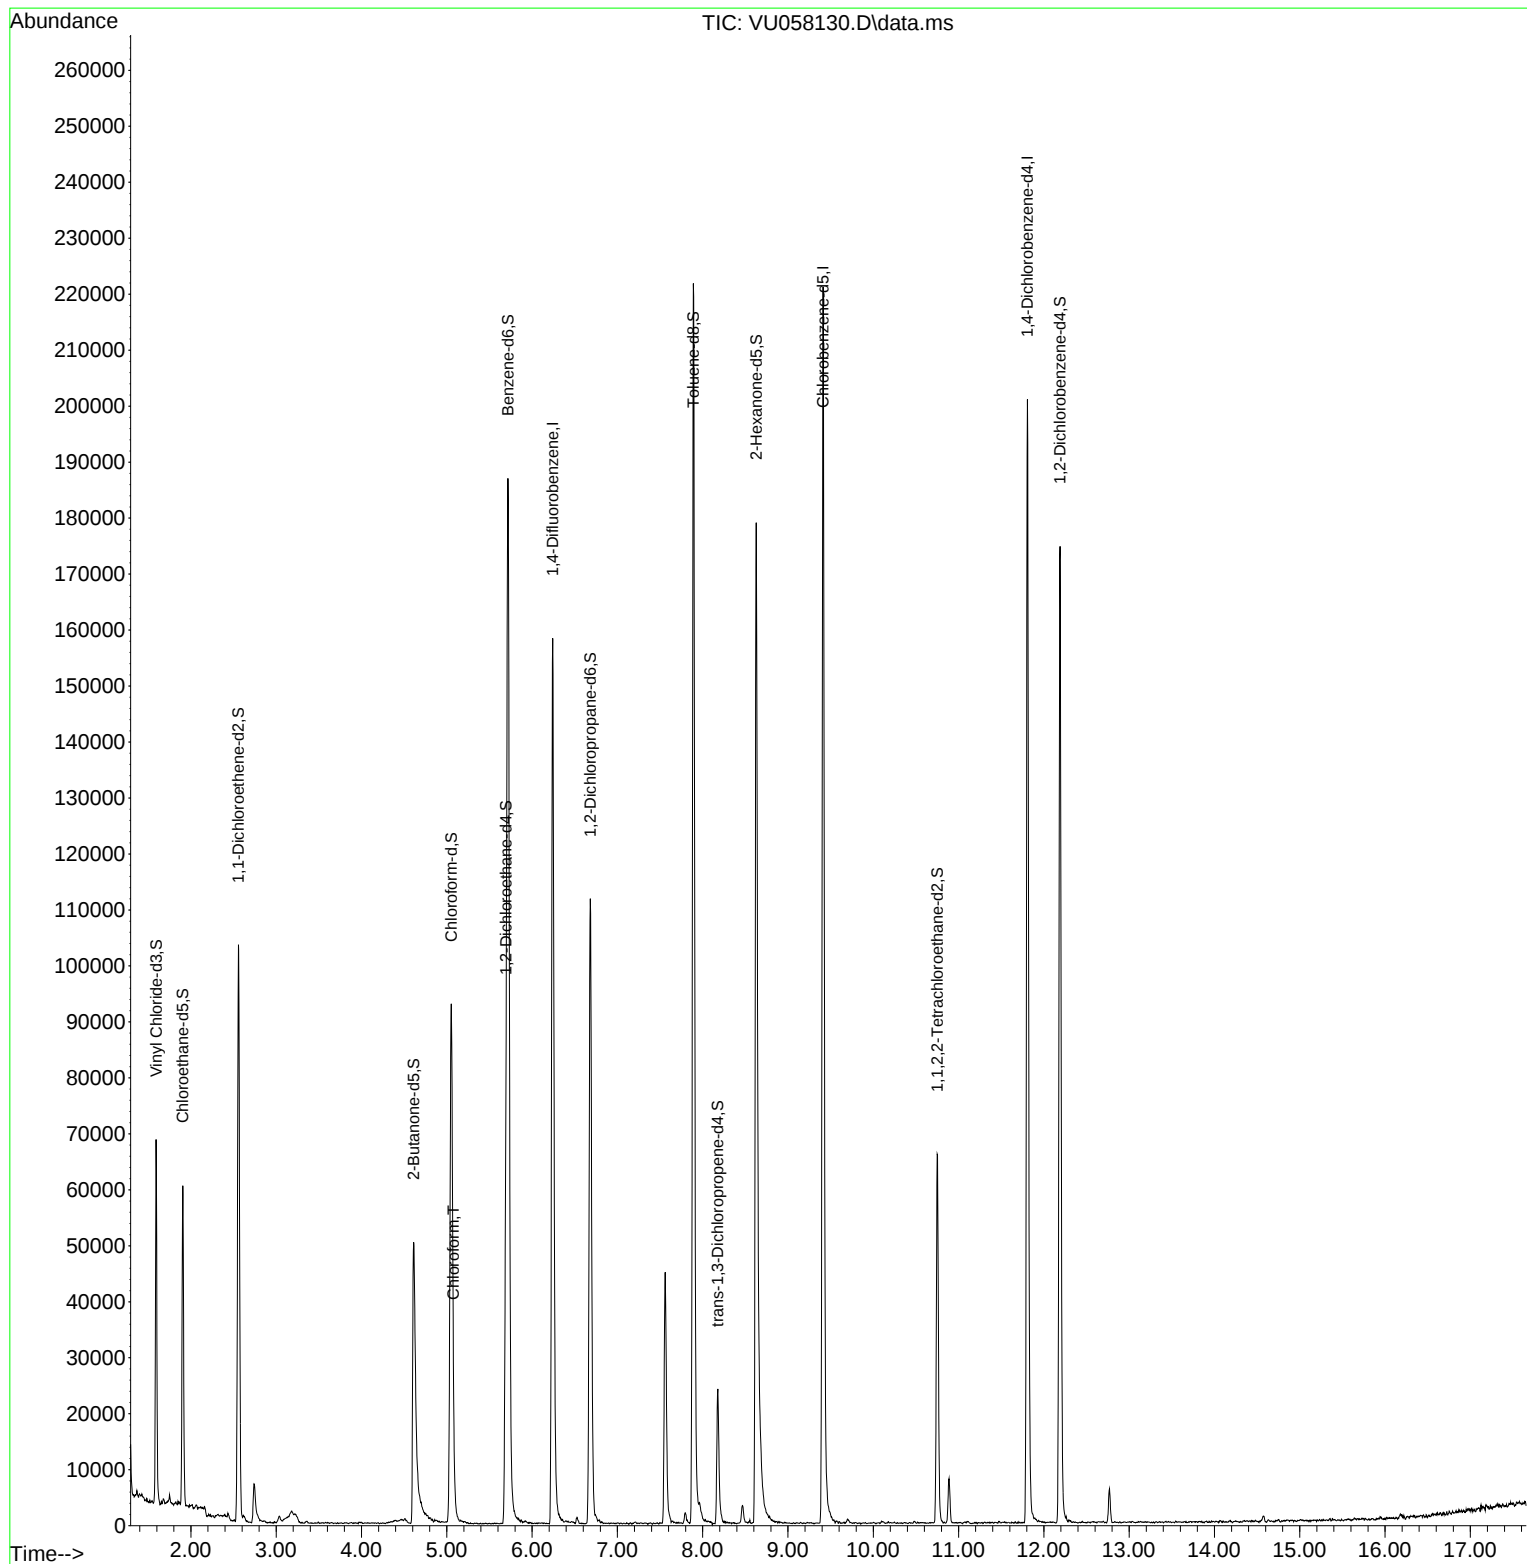

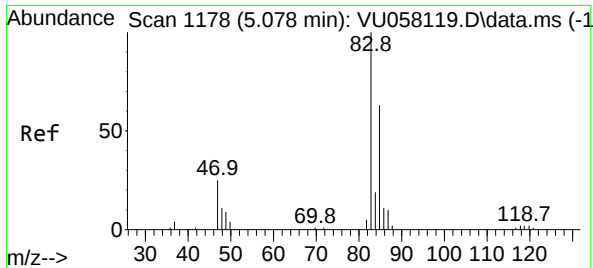

#25
 Chloroform
 Concen: 0.267 ug/L
 RT: 5.078 min Scan# 1178
 Delta R.T. 0.000 min
 Lab File: VU058130.D
 Acq: 15 Mar 2024 16:20

Instrument :
 MSVOA_U
 ClientSampleId :
 C0GP6

Tgt Ion: 83 Resp: 4544
 Ion Ratio Lower Upper
 83 100
 85 65.1 45.4 84.4

