

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031524\
 Data File : VU058126.D
 Acq On : 15 Mar 2024 14:46
 Operator : MD/SY
 Sample : P1777-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COGN6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU058126.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	87	94	111	rVB	65580	73491	15.38%	1.947%
2	1.904	183	191	203	rVB	56100	71864	15.04%	1.904%
3	2.560	382	395	410	rBV	102458	169842	35.55%	4.499%
4	2.743	441	452	462	rBV2	6150	11957	2.50%	0.317%
5	3.178	574	587	602	rBV2	5342	14376	3.01%	0.381%
6	4.612	1020	1033	1074	rBV	55476	151902	31.80%	4.024%
7	5.052	1149	1170	1195	rBV	90423	206043	43.13%	5.458%
8	5.718	1355	1377	1404	rBV2	184822	477702	100.00%	12.654%
9	6.242	1528	1540	1563	rBV	162318	315274	66.00%	8.352%
10	6.682	1661	1677	1703	rBV	113658	224893	47.08%	5.957%
11	7.560	1939	1950	1971	rBV	44527	83017	17.38%	2.199%
12	7.891	2040	2053	2074	rBV	218805	392394	82.14%	10.395%
13	8.177	2132	2142	2160	rBV	24592	43532	9.11%	1.153%
14	8.467	2220	2232	2243	rBV3	2846	5239	1.10%	0.139%
15	8.627	2272	2282	2310	rBV2	177177	372214	77.92%	9.860%
16	9.412	2511	2526	2554	rBV	223275	387642	81.15%	10.269%
17	10.750	2931	2942	2967	rVB	66181	110651	23.16%	2.931%
18	10.888	2976	2985	2998	rBV2	8392	12901	2.70%	0.342%
19	11.807	3260	3271	3294	rBV	210018	343739	71.96%	9.106%
20	12.190	3376	3390	3421	rBV	171731	297317	62.24%	7.876%
21	12.766	3561	3569	3581	rVB2	5984	9015	1.89%	0.239%




Sum of corrected areas: 3775005

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031524\
Data File : VU058126.D
Acq On : 15 Mar 2024 14:46
Operator : MD/SY
Sample : P1777-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COGN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

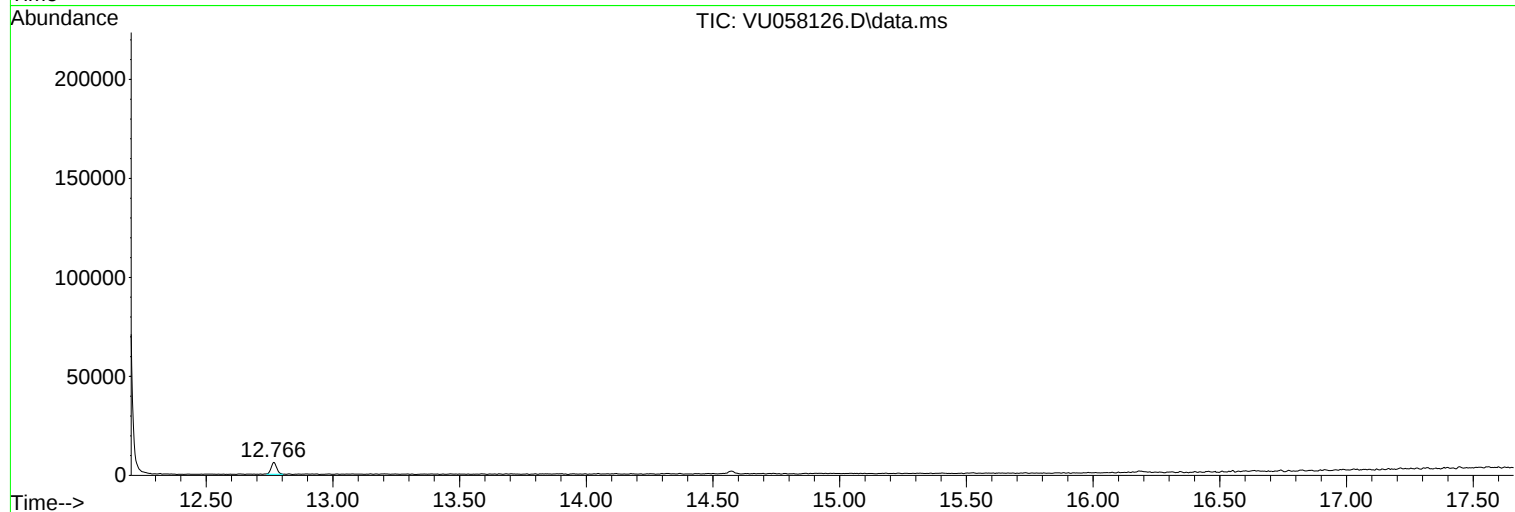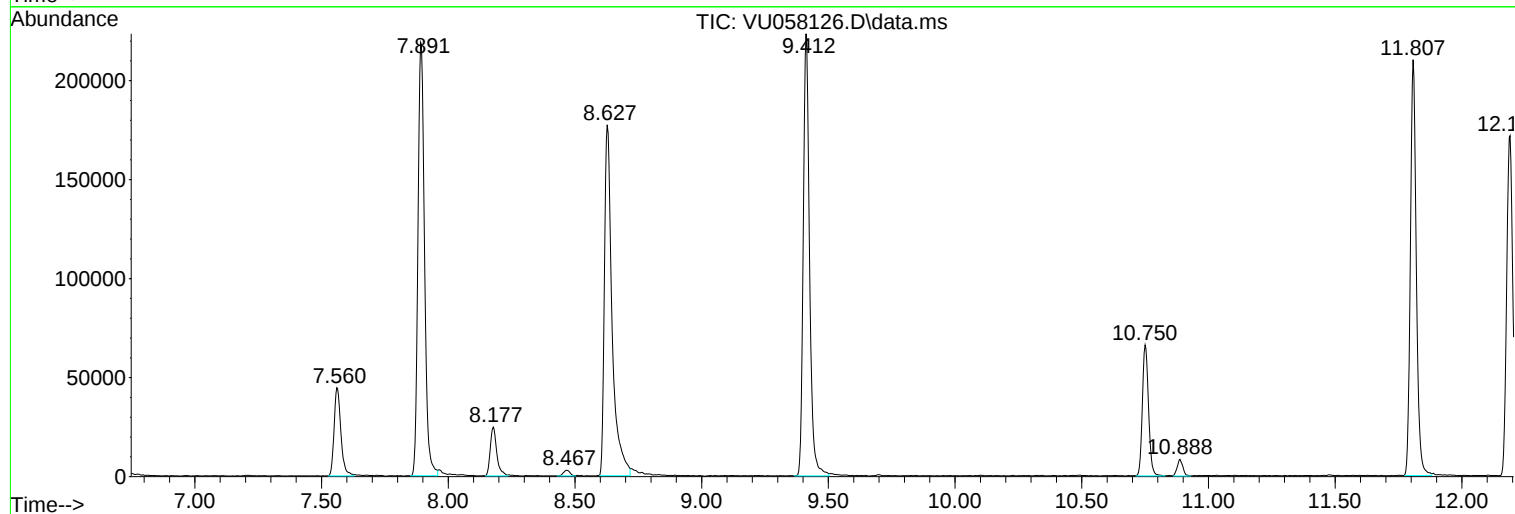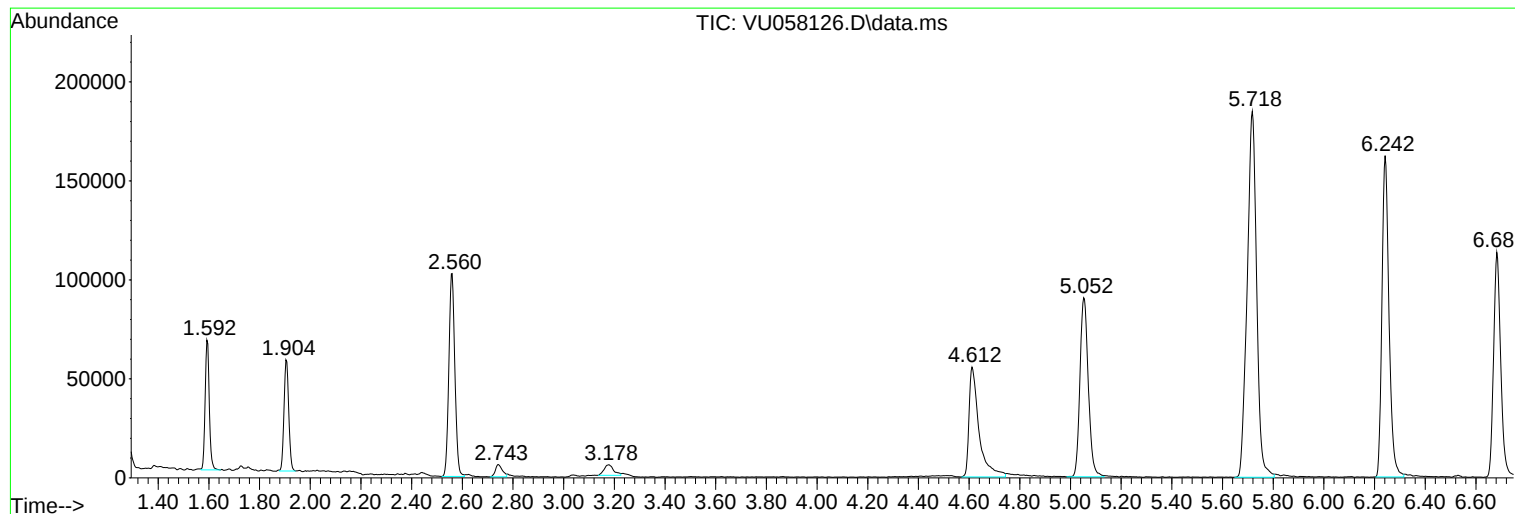

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031524\
Data File : VU058126.D
Acq On : 15 Mar 2024 14:46
Operator : MD/SY
Sample : P1777-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031524\
Data File : VU058126.D
Acq On : 15 Mar 2024 14:46
Operator : MD/SY
Sample : P1777-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COGN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc