


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031524\
Data File : VU058118.D
Acq On : 15 Mar 2024 10:13
Operator : MD/SY
Sample : BFB123
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB123

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Mar 14 04:37:22 2024

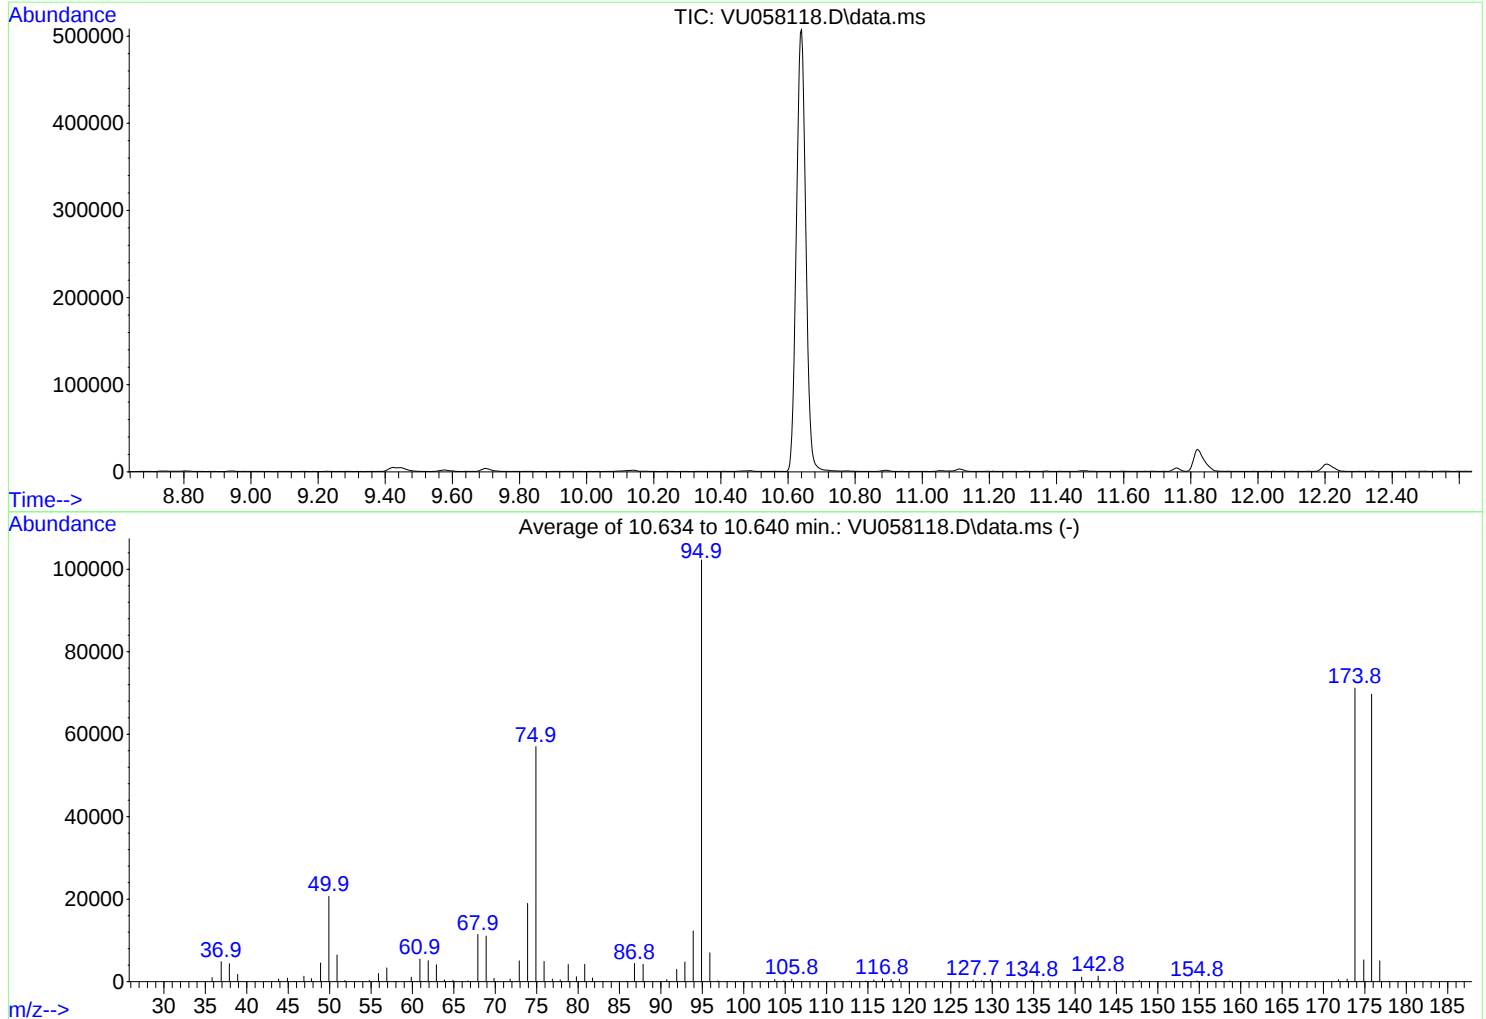

AutoFind: Scans 2906, 2907, 2908; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.2	20685	PASS
75	95	30	80	55.7	57003	PASS
95	95	100	100	100.0	102288	PASS
96	95	5	9	6.8	6985	PASS
173	174	0.00	2	0.9	632	PASS
174	95	50	120	69.6	71189	PASS
175	174	5	9	7.4	5264	PASS
176	174	95	101	98.0	69736	PASS
177	176	5	9	7.2	5043	PASS

Scan 2892 (10.589 min): VU058118.D\data.ms
BFB123

m/z	Abundance
39.80	196.0
43.90	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB123

m/z	Abundance
35.90	889.0
36.90	4639.0
37.90	4194.0
38.90	1663.0
39.90	234.0
43.90	946.0
44.90	800.0
46.90	1244.0
47.80	671.0
48.90	4399.0
49.90	20152.0
50.90	6246.0
51.90	274.0
54.80	292.0
55.90	1816.0
56.90	2944.0
57.80	140.0
59.80	1035.0
60.90	5230.0
61.90	4836.0
62.90	3962.0
63.80	464.0
64.90	298.0
66.70	178.0
67.90	10662.0
68.90	10411.0
69.90	722.0
71.80	542.0
72.90	4927.0
73.90	17816.0
74.90	54928.0
75.90	4705.0
76.90	610.0
77.80	466.0
78.80	3919.0
79.80	1195.0
80.80	4023.0
81.70	813.0
82.90	102.0
85.90	114.0
86.80	4112.0
87.80	3702.0
90.70	457.0
91.90	2766.0
92.90	4405.0
93.90	11274.0
94.90	97640.0
95.90	6723.0
96.90	236.0
103.70	518.0
104.90	234.0
105.80	511.0
112.80	145.0
114.80	167.0
115.70	385.0
116.70	619.0
117.80	465.0
118.80	603.0
127.70	350.0
128.70	195.0
129.80	316.0
130.80	131.0
134.80	271.0
136.80	221.0
140.80	1034.0
141.80	110.0
142.80	1293.0
144.70	172.0
145.70	171.0
147.80	236.0
154.80	201.0
156.90	137.0
158.70	195.0
171.80	486.0
172.80	605.0
173.80	66704.0
174.90	4963.0
175.80	65712.0
176.80	4763.0
177.90	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB123

m/z	Abundance
35.90	1001.0
36.90	4940.0
37.90	4375.0
38.90	1810.0
39.90	229.0
43.90	944.0
44.90	886.0
45.90	109.0
46.90	1290.0
47.90	746.0
48.90	4675.0
49.90	21168.0
50.90	6633.0
51.90	285.0
54.90	337.0
55.90	2010.0
56.90	3443.0
59.90	1101.0
60.90	5595.0
61.90	5182.0
62.90	4195.0
63.90	426.0
64.90	380.0
66.70	181.0
67.90	11714.0
68.90	11190.0
69.90	805.0
71.80	667.0
72.90	5151.0
73.90	19464.0
74.90	58272.0
75.90	5013.0
76.90	604.0
77.80	387.0
78.80	4231.0
79.80	1239.0
80.80	4304.0
81.70	896.0
82.90	103.0
85.90	126.0
86.80	4481.0
87.80	4304.0
90.70	525.0
91.90	3010.0
92.90	4902.0
93.90	12536.0
94.90	104744.0
95.90	7153.0
96.90	209.0
103.70	580.0
104.90	257.0
105.80	568.0
106.80	124.0
109.70	110.0
110.90	100.0
112.80	159.0
114.70	149.0
115.70	423.0
116.70	729.0
117.80	515.0
118.80	584.0
127.70	402.0
128.70	222.0
129.80	379.0
130.80	161.0
134.80	295.0
136.80	256.0
140.80	1129.0
141.70	141.0
142.80	1400.0
144.70	174.0
145.80	199.0
147.70	246.0
154.80	212.0
156.90	137.0
158.70	167.0
171.80	447.0
172.90	623.0
173.80	72464.0
174.90	5412.0
175.80	71104.0
176.80	5198.0
177.90	140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB123

m/z	Abundance
35.80	1012.0
36.90	5003.0
37.90	4448.0
38.90	1807.0
39.80	205.0
43.80	947.0
44.90	924.0
45.70	101.0
46.90	1383.0
47.80	754.0
48.90	4605.0
49.90	20736.0
50.90	6541.0
51.80	298.0
54.80	345.0
55.90	2070.0
56.90	3618.0
59.90	1144.0
60.90	5562.0
61.90	5259.0
62.90	4166.0
63.90	435.0
64.90	427.0
66.70	214.0
67.90	11939.0
68.90	11528.0
69.80	897.0
71.80	692.0
72.90	5100.0
73.90	19672.0
74.90	57808.0
75.90	4935.0
76.90	551.0
77.90	403.0
78.80	4310.0
79.80	1201.0
80.80	4247.0
81.80	922.0
85.80	152.0
86.80	4673.0
87.90	4641.0
90.70	536.0
91.90	3250.0
92.90	5045.0
93.90	13084.0
94.90	104480.0
95.90	7080.0
96.90	180.0
103.80	583.0
104.80	240.0
105.80	612.0
106.80	142.0
110.90	116.0
111.80	114.0
112.80	137.0
114.70	131.0
115.70	438.0
116.80	835.0
117.80	497.0
118.80	556.0
127.70	432.0
128.70	235.0
129.80	425.0
130.80	166.0
134.80	257.0
136.80	269.0
140.80	1189.0
141.70	156.0
142.80	1349.0
144.80	150.0
145.80	180.0
147.70	295.0
154.70	218.0
156.90	132.0
158.70	122.0
160.70	100.0
171.00	117.0
171.80	431.0
172.90	667.0
173.80	74400.0
174.80	5416.0
175.80	72392.0
176.80	5167.0
177.90	137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB123