

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031622\
 Data File : VU047588.D
 Acq On : 16 Mar 2022 14:17
 Operator : SY/MD
 Sample : N1858-23DL 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNLODL

Quant Time: Mar 17 00:51:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Mar 17 00:50:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	128007	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	127527	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	64079	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	30381	3.629	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.600%
7) Chloroethane-d5	1.919	69	34402	4.528	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.600%
11) 1,1-Dichloroethene-d2	2.571	65	13066	3.328	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.600%
20) 2-Butanone-d5	4.639	46	163608	67.922	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	135.840%#
24) Chloroform-d	5.067	84	88518	4.815	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.400%
26) 1,2-Dichloroethane-d4	5.706	65	51581	5.178	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.600%
32) Benzene-d6	5.732	84	154242	4.155	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.000%
36) 1,2-Dichloropropane-d6	6.693	67	55954	4.793	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.800%
41) Toluene-d8	7.899	98	124237	3.569	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.400%
43) trans-1,3-Dichloroprop...	8.182	79	21921	4.466	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.400%
46) 2-Hexanone-d5	8.639	63	141400	55.577	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.160%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	60627	5.200	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.000%
66) 1,2-Dichlorobenzene-d4	12.195	152	62369	4.658	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.200%
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.607	62	2628	0.330	ug/L	# 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031622\
Data File : VU047588.D
Acq On : 16 Mar 2022 14:17
Operator : SY/MD
Sample : N1858-23DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNL0DL


Quant Time: Mar 17 00:51:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Mar 17 00:50:30 2022
Response via : Initial Calibration

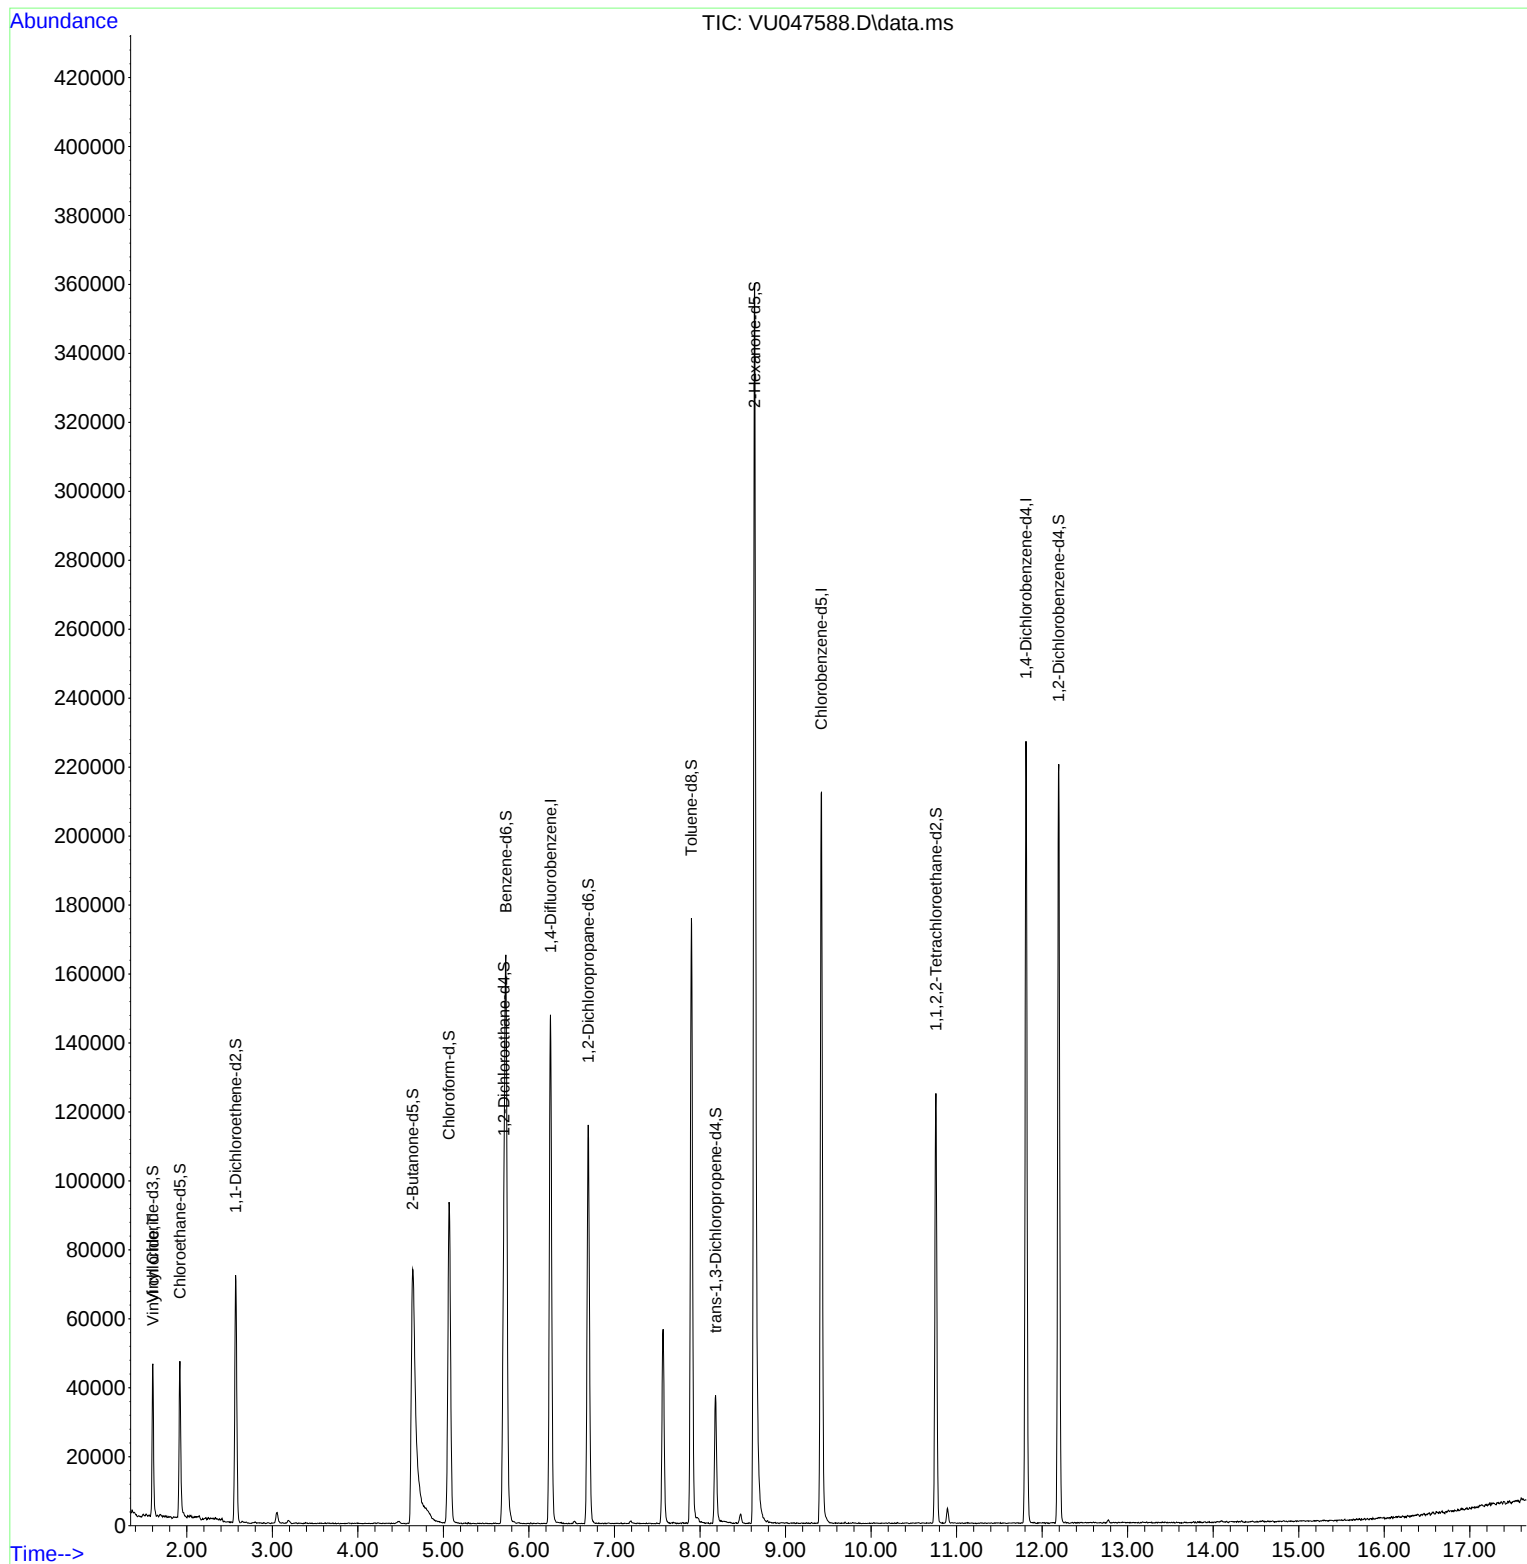

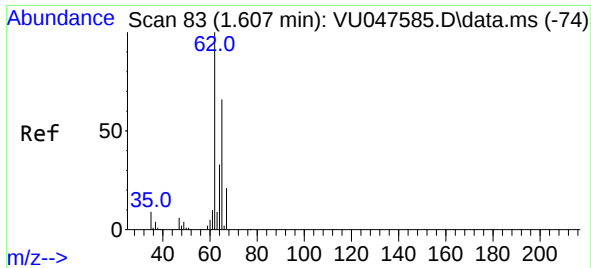

#5
Vinyl chloride
Concen: 0.330 ug/L
RT: 1.607 min Scan# 81
Delta R.T. 0.000 min
Lab File: VU047588.D
Acq: 16 Mar 2022 14:17

Instrument :
MSVOA_U
ClientSampleId :
ETNL0DL

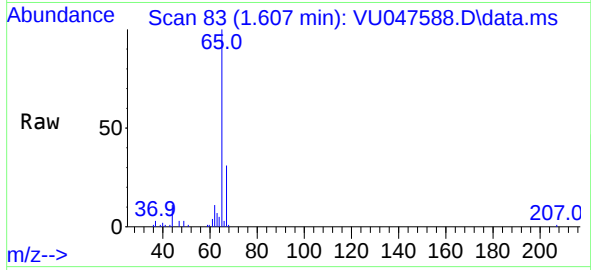

Tgt Ion: 62 Resp: 2628
Ion Ratio Lower Upper
62 100
64 44.5 23.5 43.7#

