

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031622\
 Data File : VU047586.D
 Acq On : 16 Mar 2022 12:02
 Operator : SY/MD
 Sample : VU0316WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK082

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	96	rBV	43564	49753	8.57%	1.297%
2	1.919	171	180	200	rBV	44231	61006	10.51%	1.590%
3	2.571	372	383	398	rVB	73868	119298	20.55%	3.109%
4	4.642	1011	1027	1069	rBV	62494	220313	37.95%	5.741%
5	5.067	1144	1159	1181	rBV	85981	190576	32.83%	4.966%
6	5.729	1345	1365	1388	rBV2	159585	420621	72.45%	10.961%
7	6.253	1511	1528	1551	rBV	150653	283276	48.79%	7.382%
8	6.694	1652	1665	1689	rBV	104734	207627	35.76%	5.411%
9	7.568	1924	1937	1961	rBV2	48572	86350	14.87%	2.250%
10	7.796	2001	2008	2028	rVB3	3271	6099	1.05%	0.159%
11	7.899	2028	2040	2058	rBV	173756	305401	52.61%	7.959%
12	8.182	2117	2128	2142	rBV	31670	54268	9.35%	1.414%
13	8.639	2256	2270	2307	rBV	294688	580554	100.00%	15.129%
14	9.420	2499	2513	2532	rBV	216733	359426	61.91%	9.367%
15	10.758	2914	2929	2947	rBV	100956	167384	28.83%	4.362%
16	11.812	3245	3257	3276	rVB	220571	359168	61.87%	9.360%
17	12.195	3364	3376	3393	rBV	211438	339981	58.56%	8.860%
18	13.844	3881	3889	3898	rVB4	4341	6631	1.14%	0.173%
19	14.089	3955	3965	3974	rBV	7174	10590	1.82%	0.276%
20	14.330	4032	4040	4051	rVB3	5674	9034	1.56%	0.235%




Sum of corrected areas: 3837356

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031622\
Data File : VU047586.D
Acq On : 16 Mar 2022 12:02
Operator : SY/MD
Sample : VU0316WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK082

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

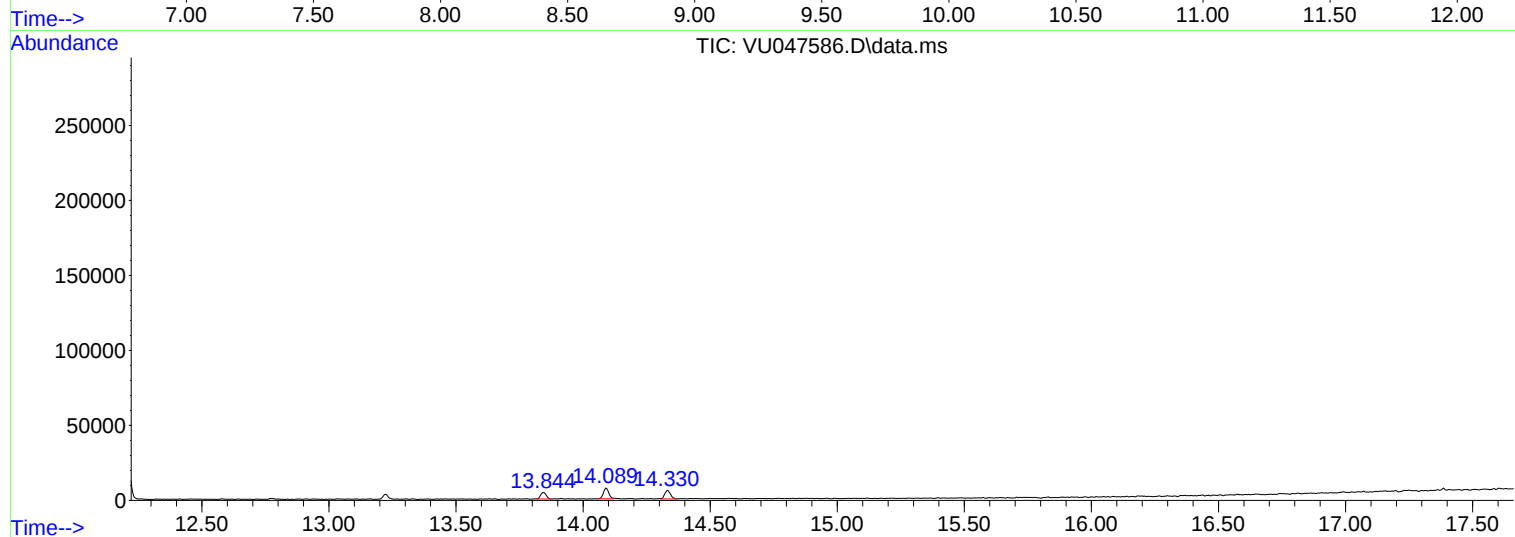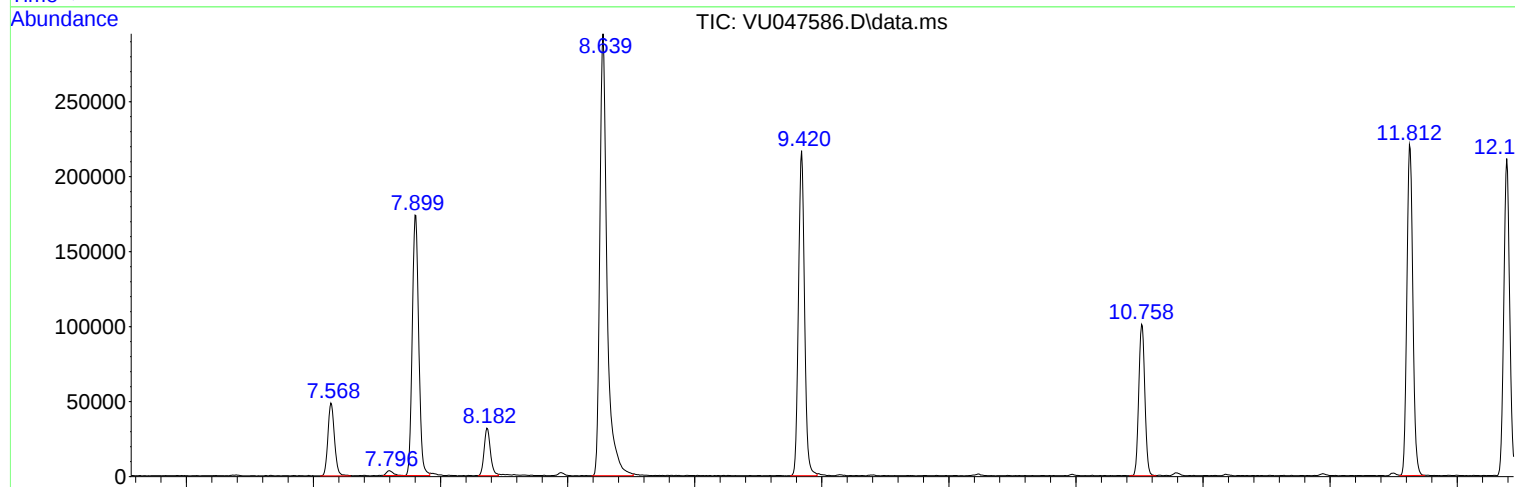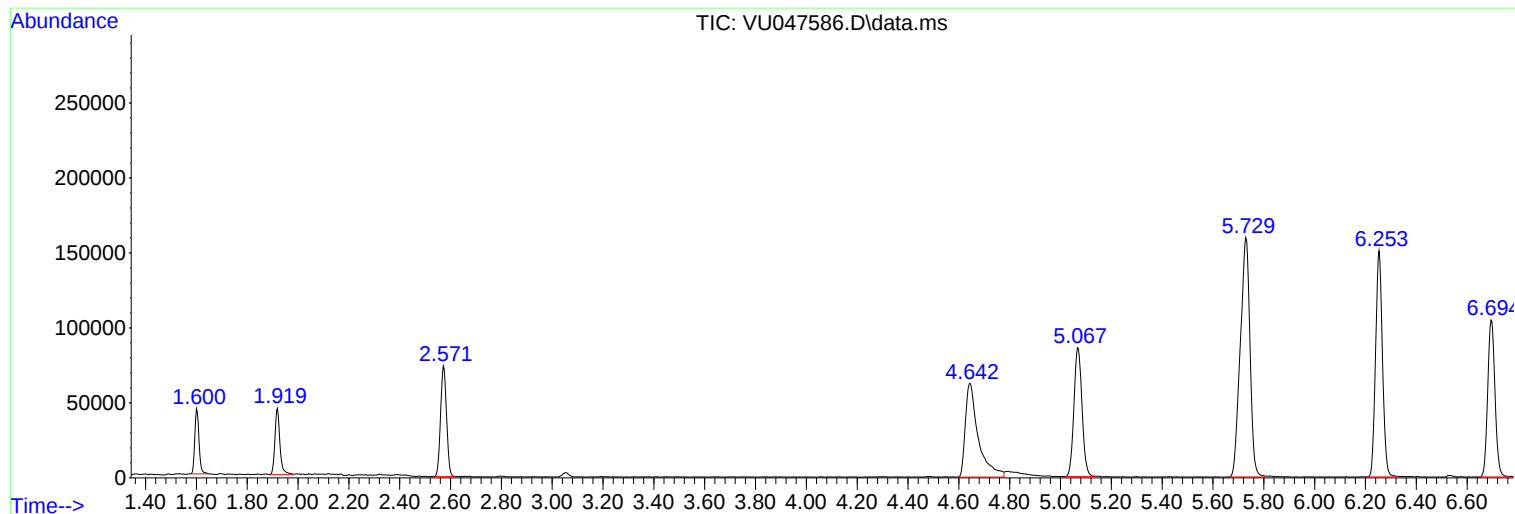

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031622\
Data File : VU047586.D
Acq On : 16 Mar 2022 12:02
Operator : SY/MD
Sample : VU0316WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK082

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031622\
Data File : VU047586.D
Acq On : 16 Mar 2022 12:02
Operator : SY/MD
Sample : VU0316WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK082

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc