


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031622\
Data File : VU047584.D
Acq On : 16 Mar 2022 09:04
Operator : SY/MD
Sample : BFB069
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB069

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Mar 18 01:27:05 2022

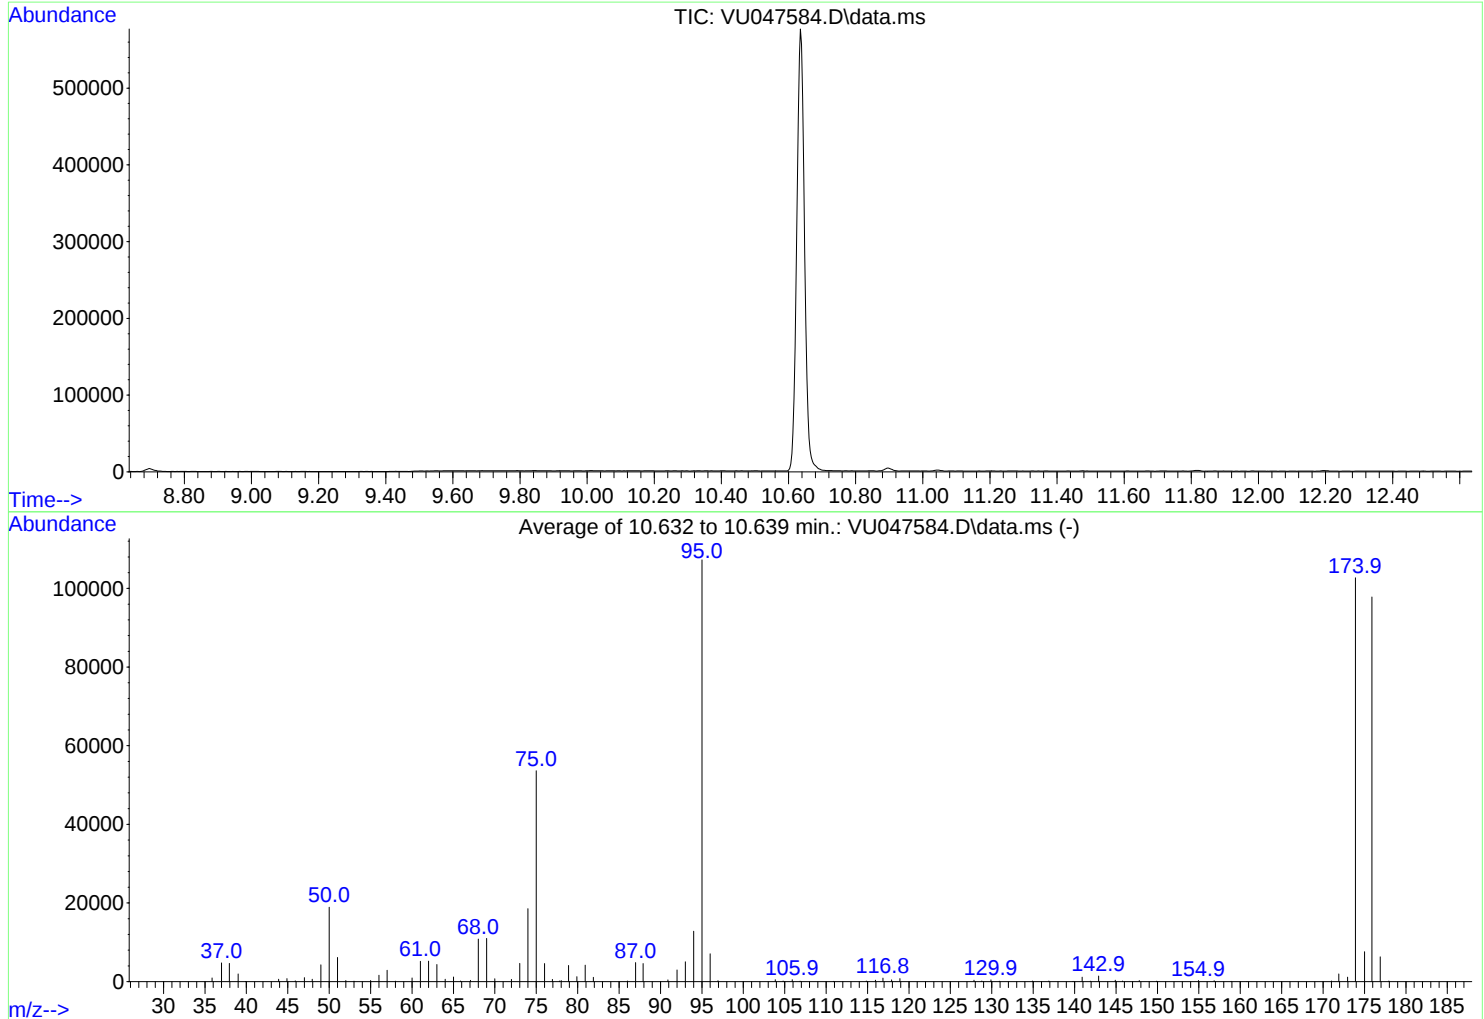

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	18939	PASS
75	95	30	80	50.0	53635	PASS
95	95	100	100	100.0	107261	PASS
96	95	5	9	6.6	7069	PASS
173	174	0.00	2	1.1	1161	PASS
174	95	50	120	95.8	102717	PASS
175	174	5	9	7.4	7616	PASS
176	174	95	101	95.2	97827	PASS
177	176	5	9	6.4	6292	PASS

m/z	Abundance
35.90	487.0
37.90	195.0
39.90	339.0
43.90	202.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069

m/z	Abundance
35.90	1388.0
37.00	4701.0
38.00	4771.0
39.00	1865.0
39.90	398.0
43.90	882.0
44.90	828.0
45.90	214.0
47.00	1017.0
47.90	580.0
49.00	4092.0
50.00	19248.0
51.00	6125.0
52.00	295.0
53.00	120.0
55.00	257.0
56.00	1602.0
57.00	2810.0
58.00	116.0
60.00	893.0
61.00	5223.0
62.00	5272.0
63.00	4284.0
64.00	604.0
65.00	1113.0
65.80	148.0
67.00	329.0
68.00	10617.0
69.00	10766.0
70.00	800.0
72.00	585.0
73.00	4538.0
74.00	17976.0
75.00	53008.0
76.00	4690.0
77.00	531.0
77.80	451.0
78.90	4139.0
79.90	1207.0
80.90	4214.0
81.90	1090.0
85.90	171.0
87.00	4696.0
87.90	4530.0
90.90	434.0
92.00	2868.0
93.00	4985.0
94.00	12521.0
95.00	104816.0
96.00	6968.0
97.00	232.0
103.90	483.0
104.80	155.0
105.90	491.0
106.90	130.0
110.90	120.0
114.80	151.0
116.00	370.0
116.80	788.0
117.90	437.0
118.90	712.0
127.80	432.0
128.90	129.0
129.90	415.0
130.90	144.0
134.90	171.0
136.90	140.0
139.80	108.0
140.90	1090.0
141.90	135.0
142.90	1335.0
144.90	395.0
145.80	148.0
147.80	265.0
149.90	102.0
154.90	296.0
156.90	242.0
171.00	163.0
171.90	1890.0
173.00	1120.0
173.90	97144.0
175.00	7399.0
175.90	92888.0
176.90	6060.0
178.00	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069

m/z	Abundance
35.90	1466.0
37.00	4937.0
38.00	4977.0
39.00	2012.0
39.90	413.0
43.90	822.0
44.90	800.0
45.90	221.0
47.00	1064.0
48.00	606.0
49.00	4418.0
50.00	19464.0
51.00	6321.0
52.00	286.0
53.00	118.0
55.00	282.0
56.00	1700.0
57.00	2987.0
58.00	125.0
60.00	958.0
61.00	5365.0
62.00	5394.0
63.00	4511.0
64.00	617.0
65.00	1209.0
65.90	148.0
67.00	353.0
68.00	11195.0
69.00	11335.0
70.00	743.0
72.00	598.0
73.00	4805.0
74.00	19208.0
75.00	55344.0
76.00	4805.0
77.00	597.0
78.00	421.0
78.90	4274.0
79.90	1309.0
80.90	4338.0
81.90	1139.0
86.00	161.0
87.00	5033.0
87.90	4754.0
90.90	444.0
92.00	3079.0
93.00	5227.0
94.00	13183.0
95.00	110832.0
96.00	7262.0
97.00	254.0
103.80	498.0
104.80	165.0
105.90	529.0
106.80	115.0
110.90	109.0
114.80	165.0
115.90	387.0
116.80	940.0
117.90	460.0
118.90	808.0
127.80	386.0
128.80	165.0
129.90	450.0
130.90	130.0
134.90	163.0
136.90	155.0
139.80	102.0
140.90	1206.0
141.90	143.0
142.90	1479.0
144.90	387.0
145.80	162.0
147.80	304.0
149.90	101.0
154.90	296.0
156.80	258.0
158.90	112.0
171.00	155.0
171.90	2011.0
173.00	1202.0
173.90	105800.0
175.00	7885.0
175.90	101184.0
176.90	6519.0
177.90	148.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069

m/z	Abundance
35.90	1433.0
37.00	4605.0
38.00	4757.0
39.00	1983.0
39.90	390.0
43.90	717.0
44.90	685.0
45.90	193.0
47.00	1016.0
48.00	613.0
49.00	4313.0
50.00	18104.0
51.00	5937.0
52.00	263.0
53.00	129.0
55.00	273.0
56.00	1608.0
57.00	2897.0
58.00	127.0
60.00	928.0
61.00	4946.0
62.00	4976.0
63.00	4327.0
64.00	597.0
65.00	1187.0
65.90	155.0
67.10	315.0
68.00	10651.0
69.00	10832.0
70.00	680.0
72.00	567.0
73.00	4577.0
74.00	18440.0
75.00	52552.0
76.00	4357.0
76.90	608.0
78.00	433.0
78.90	3898.0
79.90	1297.0
80.90	4092.0
81.90	1080.0
86.10	134.0
87.00	4840.0
87.90	4507.0
90.90	436.0
92.00	2961.0
93.00	4894.0
94.00	12754.0
95.00	106136.0
96.00	6976.0
96.90	232.0
103.80	475.0
104.80	152.0
105.90	503.0
106.80	109.0
114.90	132.0
115.90	376.0
116.90	949.0
117.90	453.0
118.90	759.0
127.90	317.0
128.70	179.0
129.90	438.0
130.90	105.0
134.90	158.0
136.90	153.0
140.90	1194.0
141.90	135.0
142.90	1468.0
144.90	334.0
145.80	159.0
147.80	305.0
149.90	114.0
155.00	271.0
156.90	228.0
158.90	116.0
160.80	106.0
171.00	121.0
171.90	1997.0
172.90	1160.0
173.90	105208.0
175.00	7564.0
175.90	99408.0
176.90	6298.0
177.90	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB069