

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031722\
 Data File : VU047605.D
 Acq On : 17 Mar 2022 13:44
 Operator : SY/MD
 Sample : N1858-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	101	rVB	76360	88763	16.05%	2.054%
2	1.919	169	180	198	rBV	54098	74952	13.55%	1.735%
3	2.572	372	383	398	rBV	119748	193725	35.02%	4.484%
4	3.054	524	533	548	rVB	3116	5637	1.02%	0.130%
5	4.642	1011	1027	1061	rBV	49958	181378	32.79%	4.198%
6	5.070	1144	1160	1183	rBV	93967	205949	37.23%	4.767%
7	5.729	1345	1365	1390	rBV2	185858	484480	87.58%	11.214%
8	6.253	1513	1528	1549	rBV	165272	312888	56.56%	7.242%
9	6.694	1652	1665	1693	rBV	113460	222690	40.26%	5.154%
10	7.571	1923	1938	1956	rBV	62242	108813	19.67%	2.519%
11	7.903	2027	2041	2058	rBV	237079	409297	73.99%	9.474%
12	7.973	2058	2063	2075	rVB3	3774	6409	1.16%	0.148%
13	8.182	2116	2128	2150	rBV	39400	69649	12.59%	1.612%
14	8.478	2208	2220	2232	rBV	4709	8912	1.61%	0.206%
15	8.639	2258	2270	2304	rBV	262150	553160	100.00%	12.803%
16	9.420	2496	2513	2533	rBV	243172	405398	73.29%	9.383%
17	10.761	2913	2930	2945	rBV	102660	169065	30.56%	3.913%
18	10.896	2962	2972	2989	rBV	8586	14070	2.54%	0.326%
19	11.816	3246	3258	3274	rBV	247739	400038	72.32%	9.259%
20	12.195	3363	3376	3396	rBV	249898	405157	73.24%	9.378%




Sum of corrected areas: 4320430

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031722\
Data File : VU047605.D
Acq On : 17 Mar 2022 13:44
Operator : SY/MD
Sample : N1858-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

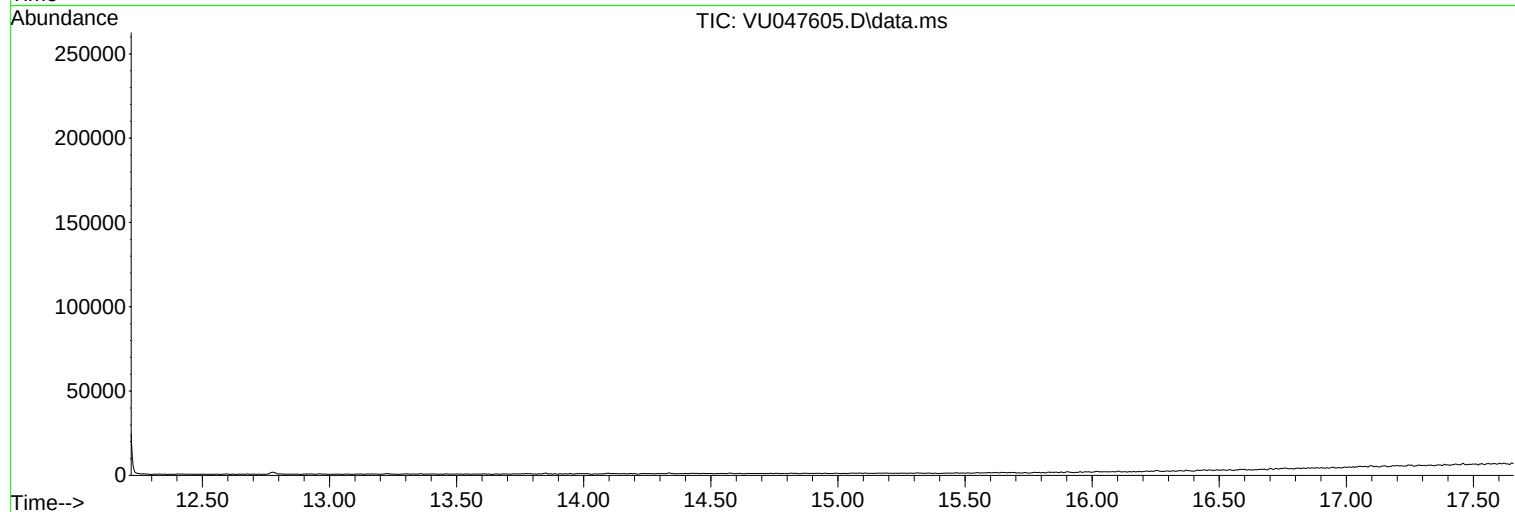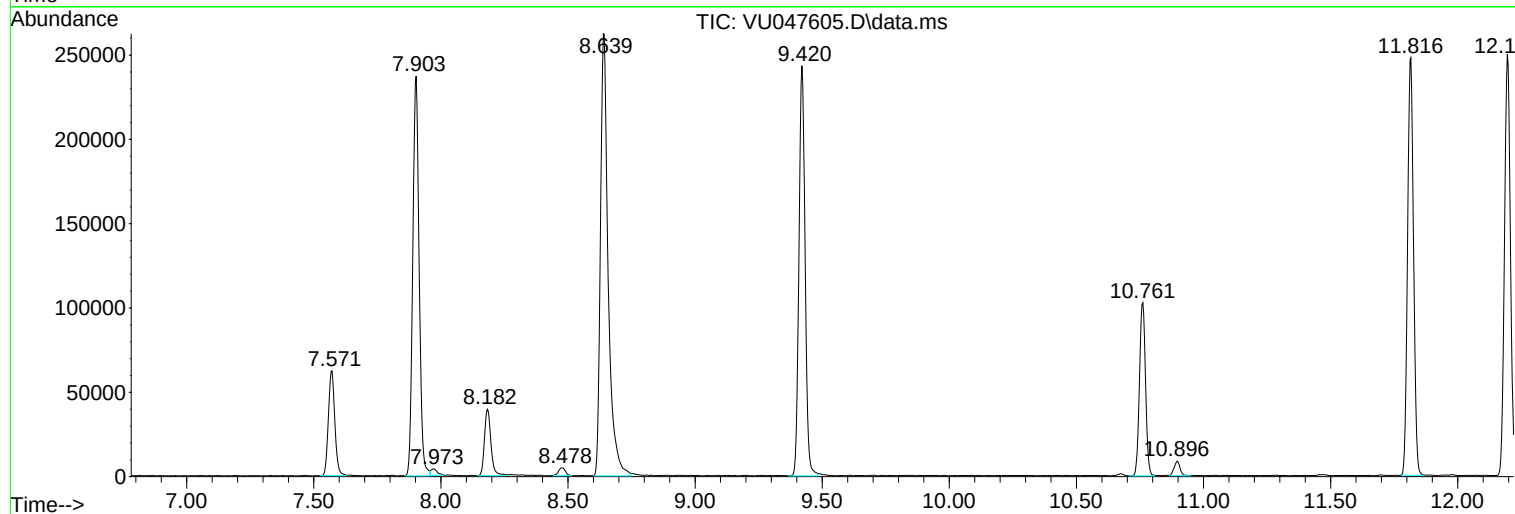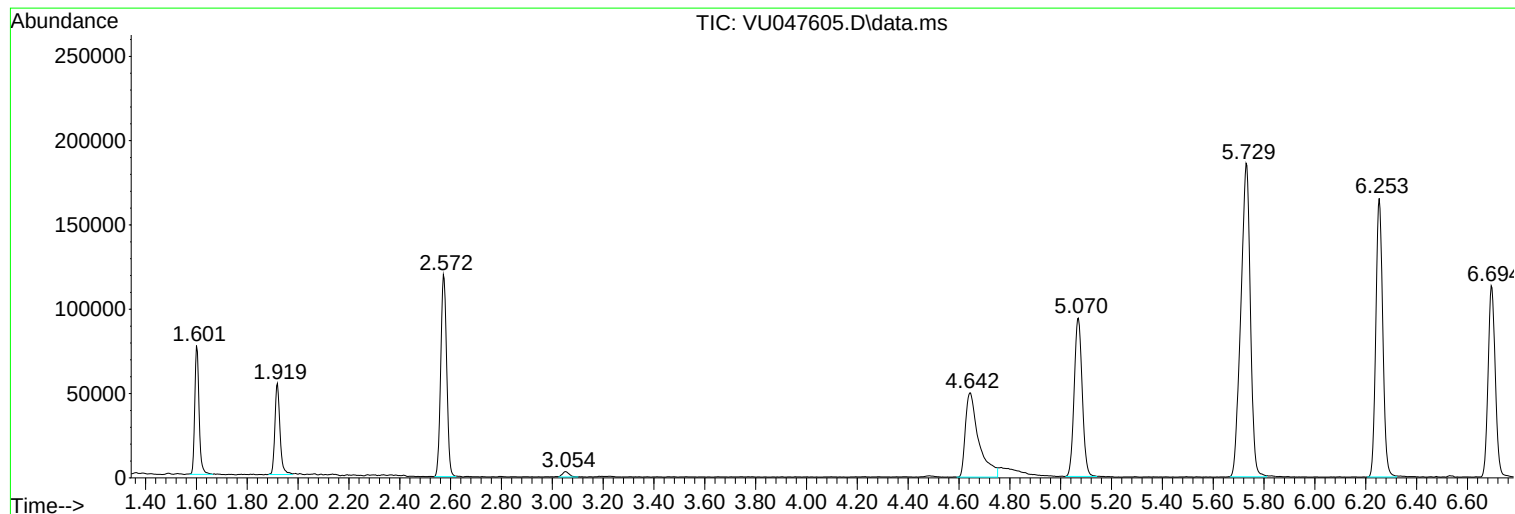

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031722\
Data File : VU047605.D
Acq On : 17 Mar 2022 13:44
Operator : SY/MD
Sample : N1858-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031722\
Data File : VU047605.D
Acq On : 17 Mar 2022 13:44
Operator : SY/MD
Sample : N1858-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc