
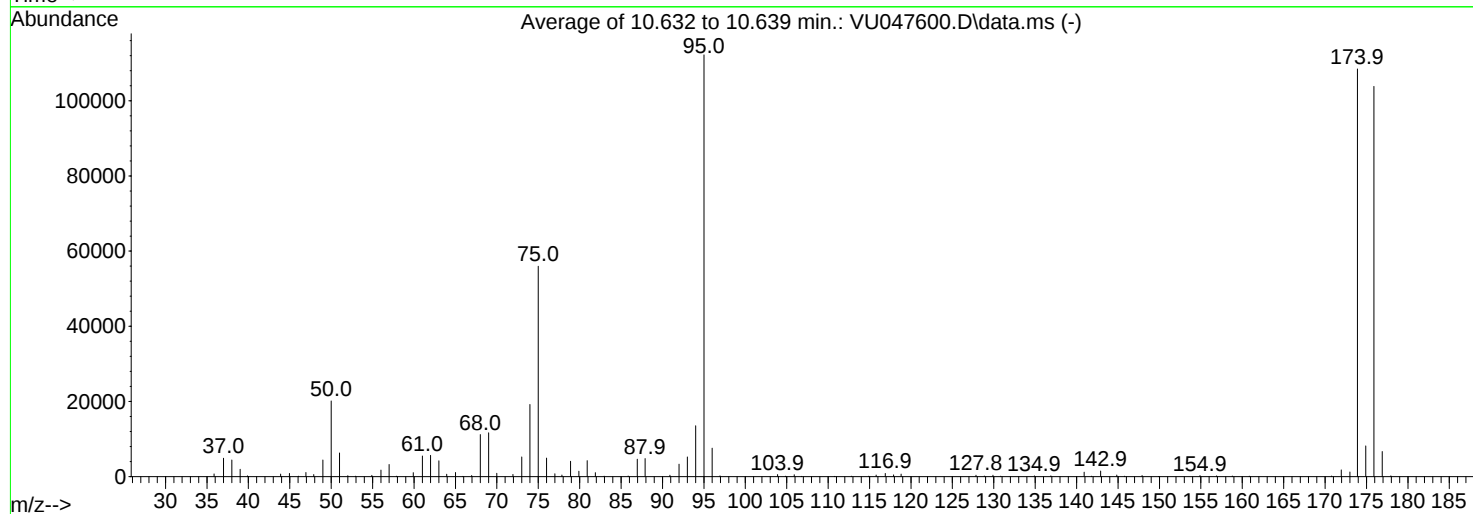


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031722\
 Data File : VU047600.D
 Acq On : 17 Mar 2022 09:15
 Operator : SY/MD
 Sample : BFB070
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB070

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Mar 18 01:27:05 2022

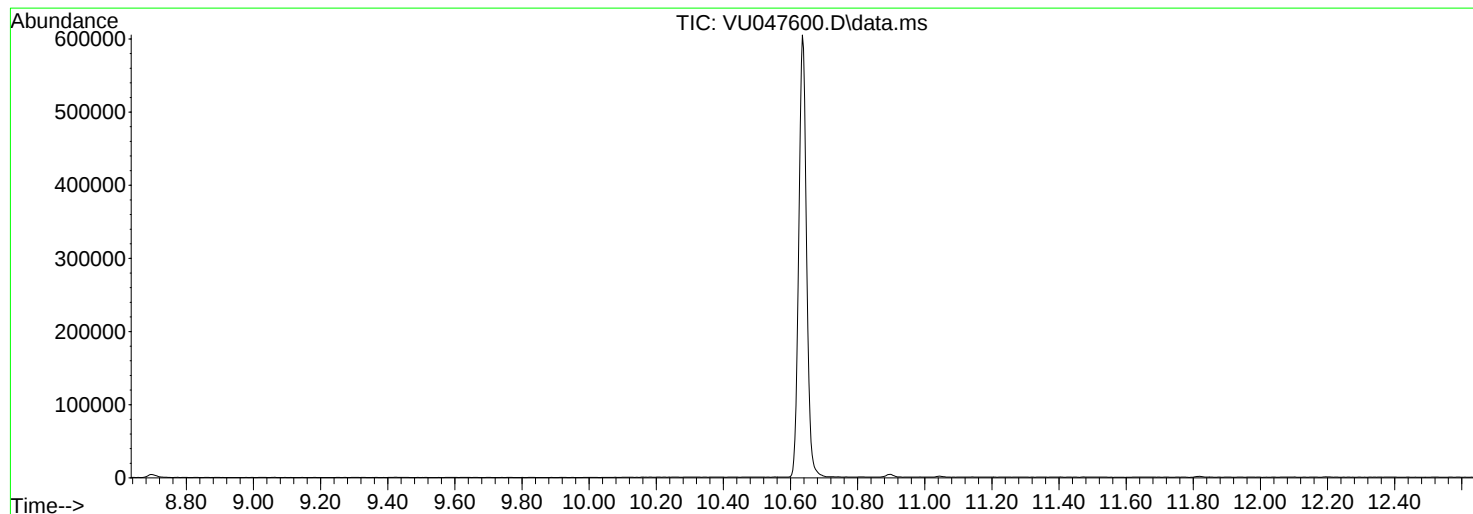

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	20136	PASS
75	95	30	80	49.9	55963	PASS
95	95	100	100	100.0	112213	PASS
96	95	5	9	6.7	7569	PASS
173	174	0.00	2	1.1	1220	PASS
174	95	50	120	96.7	108483	PASS
175	174	5	9	7.5	8188	PASS
176	174	95	101	95.7	103808	PASS
177	176	5	9	6.5	6697	PASS

m/z	Abundance
35.90	438.0
38.00	133.0
39.90	339.0
43.90	205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070

m/z	Abundance
35.90	1193.0
37.00	4801.0
38.00	4458.0
39.00	2017.0
39.90	523.0
43.90	919.0
45.00	790.0
46.00	132.0
47.00	1119.0
47.90	539.0
49.00	4238.0
50.00	19848.0
51.00	6289.0
52.00	291.0
52.90	180.0
54.90	295.0
56.00	1662.0
57.00	3170.0
57.90	158.0
59.90	1094.0
61.00	5486.0
62.00	5602.0
63.00	4357.0
63.90	606.0
65.00	1159.0
65.90	108.0
67.00	301.0
68.00	11137.0
69.00	11406.0
70.00	849.0
71.90	568.0
73.00	5161.0
74.00	18840.0
75.00	54328.0
76.00	4970.0
77.00	690.0
77.90	445.0
78.90	4108.0
79.90	1365.0
80.90	4182.0
81.90	1039.0
83.00	122.0
85.90	186.0
87.00	4599.0
87.90	4857.0
90.90	367.0
92.00	3295.0
93.00	5142.0
94.00	13390.0
95.00	109216.0
96.00	7667.0
97.00	204.0
103.90	496.0
104.90	149.0
105.90	507.0
112.80	112.0
114.90	113.0
115.80	402.0
116.90	854.0
117.90	401.0
118.80	645.0
127.80	409.0
128.90	187.0
129.90	361.0
130.90	135.0
134.90	212.0
136.90	165.0
140.90	1117.0
141.80	108.0
142.90	1451.0
144.90	445.0
145.80	115.0
147.90	278.0
154.90	282.0
156.90	218.0
158.80	148.0
160.80	138.0
170.80	204.0
171.90	1769.0
173.00	1267.0
173.90	102432.0
174.90	7818.0
175.90	98320.0
176.90	6440.0
178.00	169.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070

m/z	Abundance
35.90	1162.0
37.00	5024.0
38.00	4733.0
39.00	2009.0
39.90	573.0
43.90	924.0
44.90	859.0
46.10	146.0
46.90	1105.0
47.90	563.0
49.00	4577.0
50.00	20720.0
51.00	6542.0
52.00	299.0
53.00	145.0
54.90	343.0
56.00	1817.0
57.00	3317.0
57.90	134.0
59.90	1118.0
61.00	5671.0
62.00	5868.0
63.00	4306.0
63.90	672.0
65.00	1146.0
65.90	100.0
66.90	327.0
68.00	11558.0
69.00	12142.0
70.00	930.0
71.90	591.0
73.00	5451.0
74.00	19784.0
75.00	57928.0
76.00	5090.0
77.00	792.0
77.90	464.0
78.90	4237.0
79.90	1481.0
80.90	4387.0
81.90	1075.0
82.90	136.0
85.80	202.0
86.90	4749.0
87.90	4907.0
90.90	379.0
92.00	3444.0
93.00	5401.0
94.00	14023.0
95.00	115688.0
96.00	7890.0
97.00	230.0
103.90	592.0
104.90	147.0
105.90	539.0
106.80	103.0
110.80	108.0
112.80	113.0
114.90	115.0
115.80	415.0
116.90	882.0
117.90	477.0
118.80	683.0
127.80	385.0
128.90	179.0
129.90	374.0
130.80	137.0
134.90	241.0
136.90	200.0
140.90	1216.0
141.80	140.0
142.90	1548.0
144.80	441.0
145.80	117.0
147.90	281.0
149.90	104.0
154.90	303.0
156.90	226.0
158.80	156.0
160.80	149.0
170.80	195.0
171.90	1868.0
173.00	1259.0
173.90	111968.0
174.90	8470.0
175.90	106960.0
176.90	6904.0
178.00	205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070

m/z	Abundance
35.90	1129.0
37.00	4844.0
38.00	4546.0
39.00	1794.0
39.90	562.0
44.00	845.0
44.90	847.0
46.10	141.0
46.90	1048.0
47.90	571.0
49.00	4417.0
50.00	19840.0
51.00	6112.0
52.00	246.0
53.00	126.0
54.90	367.0
56.00	1795.0
57.00	3179.0
57.90	106.0
59.90	1044.0
61.00	5370.0
62.00	5486.0
63.00	4019.0
64.00	644.0
65.00	1027.0
66.90	338.0
68.00	10847.0
69.00	11449.0
70.00	950.0
72.00	609.0
73.00	5125.0
74.00	18944.0
75.00	55632.0
76.00	4823.0
77.00	792.0
77.80	445.0
78.90	3979.0
79.90	1450.0
80.90	4217.0
81.90	1058.0
82.90	147.0
85.80	190.0
86.90	4538.0
87.90	4633.0
90.90	364.0
92.00	3204.0
93.00	5147.0
94.00	13265.0
95.00	111736.0
96.00	7149.0
96.90	221.0
103.90	633.0
104.80	152.0
105.90	533.0
106.80	108.0
110.80	147.0
112.80	107.0
114.90	106.0
115.80	443.0
116.90	845.0
117.90	497.0
118.80	685.0
127.90	335.0
128.80	169.0
129.90	364.0
130.90	132.0
134.90	250.0
136.90	233.0
140.90	1234.0
141.80	144.0
142.90	1496.0
144.90	376.0
145.80	131.0
147.90	287.0
154.90	283.0
156.90	216.0
158.80	152.0
160.90	144.0
170.80	154.0
172.00	1750.0
173.00	1133.0
173.90	111048.0
174.90	8275.0
175.90	106144.0
176.90	6747.0
177.90	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB070