

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031725\
 Data File : VU063295.D
 Acq On : 17 Mar 2025 15:49
 Operator : MD/SY
 Sample : VU0317WBL01
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK115

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031725WMA.M
 Title : VOC Analysis

Signal : TIC: VU063295.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	86	94	111	rBV	159569	182770	14.60%	1.998%
2	1.782	136	153	163	rBV4	24590	52902	4.23%	0.578%
3	1.898	180	189	206	rVB	124489	170184	13.60%	1.860%
4	2.554	381	393	410	rBV	252104	412618	32.96%	4.510%
5	2.782	455	464	479	rVB2	6387	10748	0.86%	0.117%
6	2.843	479	483	487	rBV2	336	265	0.02%	0.003%
7	3.030	532	541	551	rBV4	2016	3414	0.27%	0.037%
8	3.174	573	586	599	rBV2	5899	14041	1.12%	0.153%
9	3.290	618	622	627	rBV	250	274	0.02%	0.003%
10	3.348	630	640	656	rVB6	2917	5963	0.48%	0.065%
11	3.422	660	663	672	rVB2	234	302	0.02%	0.003%
12	3.493	680	685	688	rVB2	221	205	0.02%	0.002%
13	3.788	771	777	781	rBV	261	248	0.02%	0.003%
14	3.985	835	838	843	rBV2	187	184	0.01%	0.002%
15	4.014	843	847	854	rVB2	205	221	0.02%	0.002%
16	4.342	938	949	951	rBV2	195	280	0.02%	0.003%
17	4.374	956	959	965	rVV2	199	184	0.01%	0.002%
18	4.608	1023	1032	1066	rBV	112820	289449	23.12%	3.164%
19	5.049	1154	1169	1201	rBV	215352	485803	38.81%	5.310%
20	5.235	1223	1227	1229	rVB	373	260	0.02%	0.003%
21	5.255	1229	1233	1240	rVB3	355	415	0.03%	0.005%
22	5.293	1240	1245	1247	rBV	267	253	0.02%	0.003%
23	5.348	1259	1262	1264	rBV	250	179	0.01%	0.002%
24	5.377	1267	1271	1272	rBV2	344	206	0.02%	0.002%
25	5.502	1308	1310	1314	rBV3	457	250	0.02%	0.003%
26	5.711	1356	1375	1416	rBV2	458479	1251788	100.00%	13.683%
27	5.946	1446	1448	1450	rBV	276	184	0.01%	0.002%
28	5.972	1454	1456	1459	rVV3	387	255	0.02%	0.003%
29	5.997	1461	1464	1468	rVV	289	197	0.02%	0.002%
30	6.020	1468	1471	1473	rVV	330	236	0.02%	0.003%
31	6.033	1473	1475	1479	rVV2	430	370	0.03%	0.004%
32	6.052	1479	1481	1483	rVV2	408	202	0.02%	0.002%
33	6.068	1483	1486	1491	rVB	351	344	0.03%	0.004%
34	6.136	1503	1507	1515	rVB2	198	229	0.02%	0.003%
35	6.239	1526	1539	1567	rBV	342146	672762	53.74%	7.354%
36	6.431	1595	1599	1605	rVB2	570	595	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031725\
 Data File : VU063295.D
 Acq On : 17 Mar 2025 15:49
 Operator : MD/SY
 Sample : VU0317WBL01
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK115

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031725WMA.M
 Title : VOC Analysis

37	6.538	1620	1632	1645	rVB9	5143	11374	0.91%	0.124%
38	6.612	1653	1655	1660	rVB2	254	193	0.02%	0.002%
39	6.679	1660	1676	1702	rBV	284163	562450	44.93%	6.148%
40	6.849	1727	1729	1732	rVB2	491	210	0.02%	0.002%
41	6.869	1732	1735	1742	rVB2	183	228	0.02%	0.002%
42	6.930	1748	1754	1755	rBV2	224	192	0.02%	0.002%
43	7.030	1776	1785	1793	rBV2	234	468	0.04%	0.005%
44	7.100	1802	1807	1811	rBV2	398	499	0.04%	0.005%
45	7.197	1829	1837	1845	rBV3	1602	2622	0.21%	0.029%
46	7.370	1888	1891	1896	rVB	248	210	0.02%	0.002%
47	7.402	1896	1901	1905	rVB2	279	227	0.02%	0.002%
48	7.557	1937	1949	1976	rBV	146991	269432	21.52%	2.945%
49	7.711	1992	1997	2003	rBV4	750	792	0.06%	0.009%
50	7.737	2003	2005	2012	rVB4	538	565	0.05%	0.006%
51	7.795	2016	2023	2033	rVB5	1370	2480	0.20%	0.027%
52	7.888	2040	2052	2074	rBV	548411	940014	75.09%	10.275%
53	8.171	2128	2140	2165	rBV	102820	184577	14.75%	2.018%
54	8.329	2185	2189	2194	rBV3	289	310	0.02%	0.003%
55	8.402	2209	2212	2220	rVB3	278	256	0.02%	0.003%
56	8.505	2242	2244	2249	rVB2	287	183	0.01%	0.002%
57	8.550	2249	2258	2266	rVB7	2944	4426	0.35%	0.048%
58	8.621	2270	2280	2322	rBV	284366	583341	46.60%	6.376%
59	9.049	2409	2413	2415	rBV3	261	233	0.02%	0.003%
60	9.113	2429	2433	2435	rBV2	231	189	0.02%	0.002%
61	9.409	2512	2525	2567	rBV	492244	857241	68.48%	9.370%
62	9.563	2567	2573	2583	rVB4	2285	3377	0.27%	0.037%
63	9.647	2596	2599	2606	rVB3	480	514	0.04%	0.006%
64	9.695	2606	2614	2627	rBV4	1789	3294	0.26%	0.036%
65	9.814	2647	2651	2654	rBV	288	248	0.02%	0.003%
66	10.103	2731	2741	2746	rBV4	2404	3419	0.27%	0.037%
67	10.364	2818	2822	2824	rBV2	223	187	0.01%	0.002%
68	10.435	2841	2844	2850	rBV2	182	197	0.02%	0.002%
69	10.483	2850	2859	2869	rVB3	1758	2461	0.20%	0.027%
70	10.534	2872	2875	2882	rVB	281	235	0.02%	0.003%
71	10.605	2892	2897	2901	rBV2	353	337	0.03%	0.004%
72	10.746	2927	2941	2960	rBV	374283	625945	50.00%	6.842%
73	10.936	2997	3000	3006	rBV2	180	226	0.02%	0.002%
74	11.087	3041	3047	3052	rBV3	1346	1788	0.14%	0.020%
75	11.197	3075	3081	3086	rVB2	316	333	0.03%	0.004%
76	11.225	3086	3090	3095	rBV2	258	299	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031725\
 Data File : VU063295.D
 Acq On : 17 Mar 2025 15:49
 Operator : MD/SY
 Sample : VU0317WBL01
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK115

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031725WMA.M
 Title : VOC Analysis

77	11.415	3145	3149	3152	rBV	375	319	0.03%	0.003%
78	11.470	3157	3166	3172	rBV4	2392	3522	0.28%	0.038%
79	11.605	3204	3208	3213	rBV	206	299	0.02%	0.003%
80	11.743	3243	3251	3258	rBV4	5299	8030	0.64%	0.088%
81	11.804	3258	3270	3296	rVV	398671	692293	55.30%	7.567%
82	12.000	3329	3331	3334	rVB	451	245	0.02%	0.003%
83	12.184	3375	3388	3414	rBV	436035	746616	59.64%	8.161%
84	12.367	3442	3445	3448	rBV4	465	329	0.03%	0.004%
85	12.451	3468	3471	3479	rVB2	369	366	0.03%	0.004%
86	12.534	3493	3497	3504	rVB2	411	456	0.04%	0.005%
87	12.730	3555	3558	3562	rVB	394	220	0.02%	0.002%
88	12.753	3562	3565	3568	rBV3	340	244	0.02%	0.003%
89	12.933	3617	3621	3623	rBV	217	187	0.01%	0.002%
90	13.004	3638	3643	3647	rBV4	822	896	0.07%	0.010%
91	13.116	3675	3678	3681	rVB	320	220	0.02%	0.002%
92	13.222	3703	3711	3724	rBV5	4666	8376	0.67%	0.092%
93	13.663	3842	3848	3851	rBV3	336	330	0.03%	0.004%
94	13.846	3896	3905	3916	rBV4	9155	15160	1.21%	0.166%
95	14.000	3950	3953	3955	rBV2	386	287	0.02%	0.003%
96	14.016	3956	3958	3961	rVB2	333	225	0.02%	0.002%
97	14.094	3973	3982	4001	rBV2	12491	28329	2.26%	0.310%
98	14.161	4001	4003	4008	rVB2	701	545	0.04%	0.006%
99	14.328	4046	4055	4069	rBV3	9959	16347	1.31%	0.179%
100	14.659	4156	4158	4161	rBV	387	266	0.02%	0.003%




Sum of corrected areas: 9148459

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031725\
Data File : VU063295.D
Acq On : 17 Mar 2025 15:49
Operator : MD/SY
Sample : VU0317WBL01
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK115

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

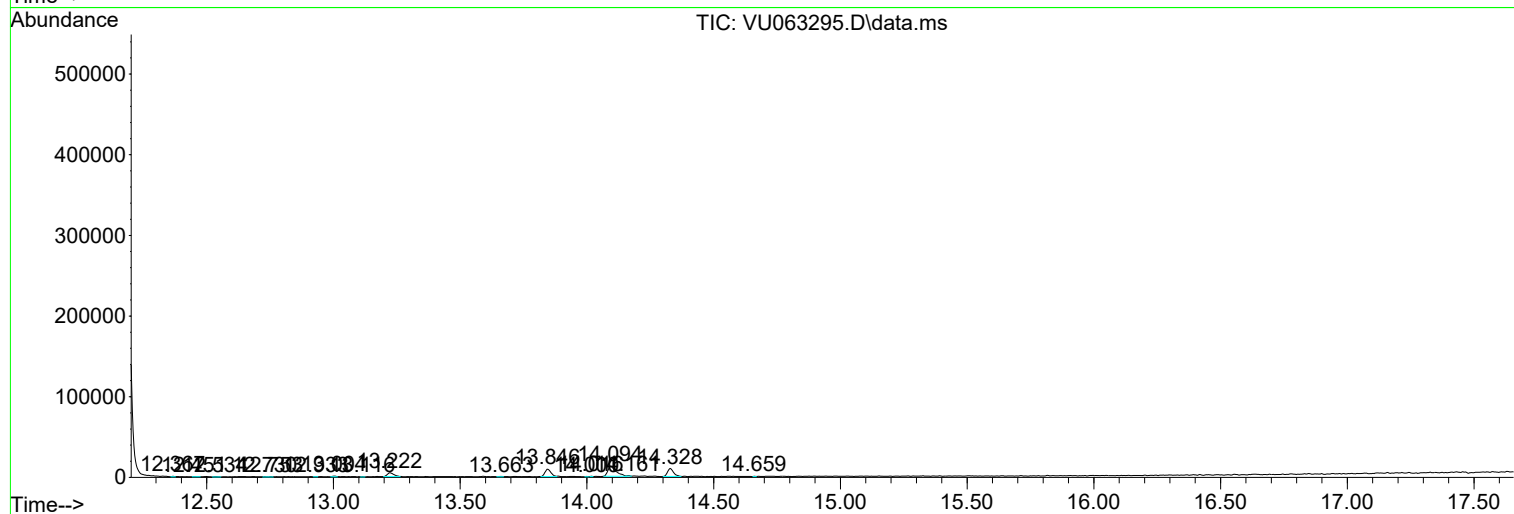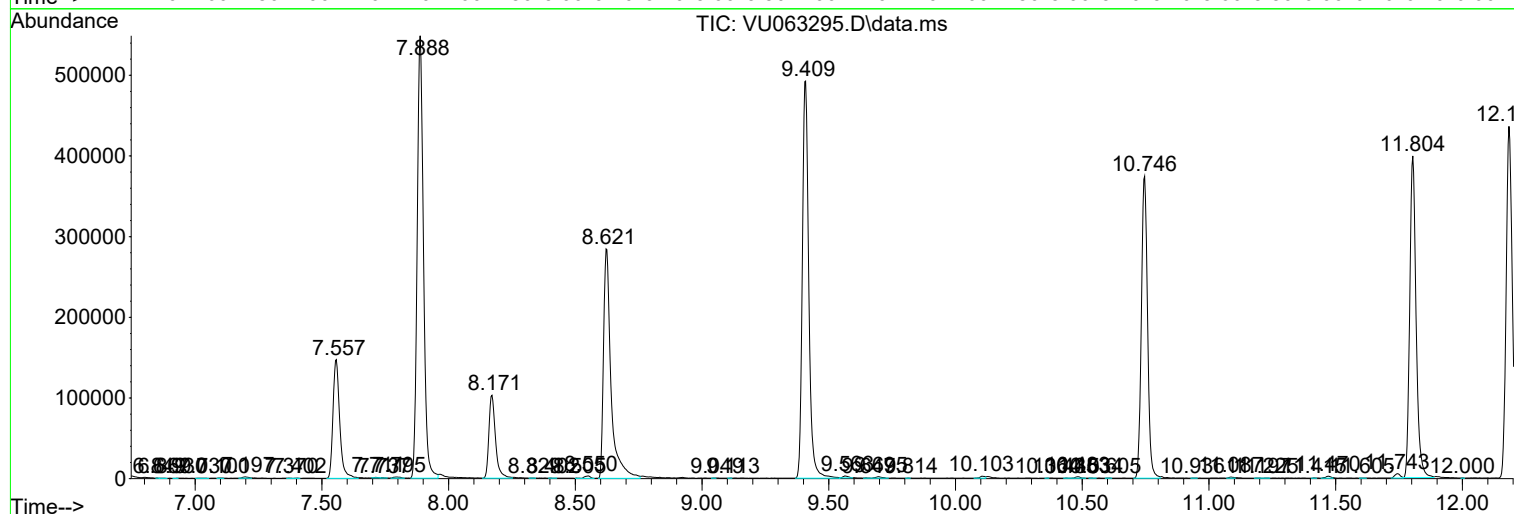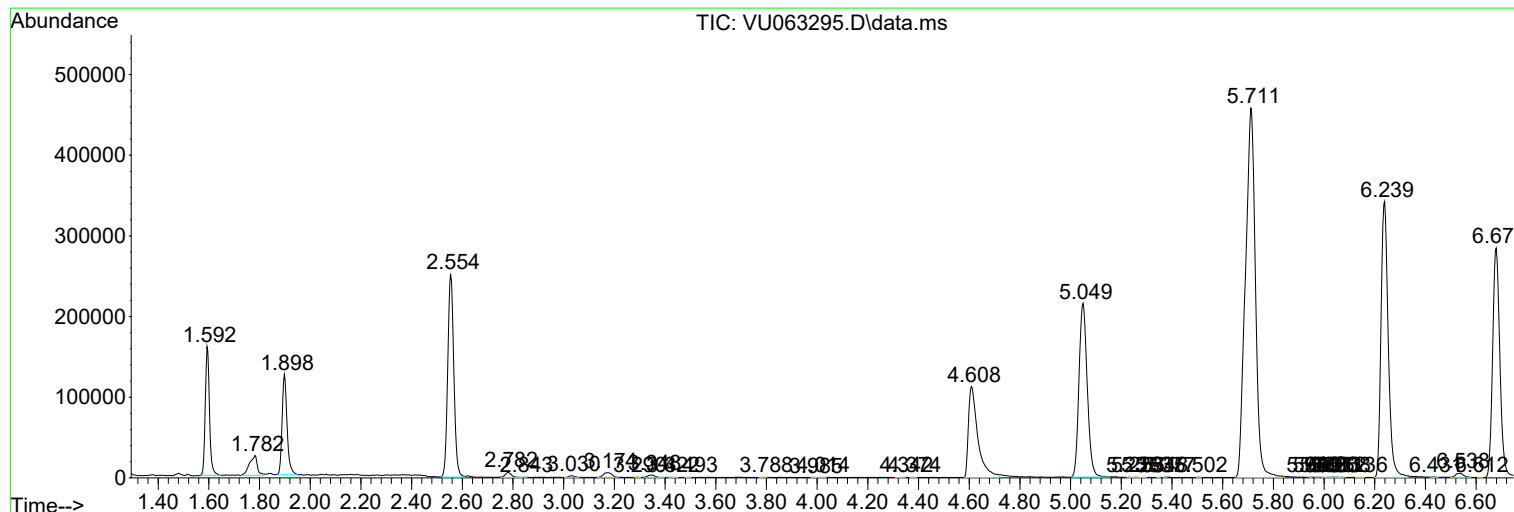

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031725\
Data File : VU063295.D
Acq On : 17 Mar 2025 15:49
Operator : MD/SY
Sample : VU0317WBL01
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK115

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031725\
Data File : VU063295.D
Acq On : 17 Mar 2025 15:49
Operator : MD/SY
Sample : VU0317WBL01
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK115

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------