
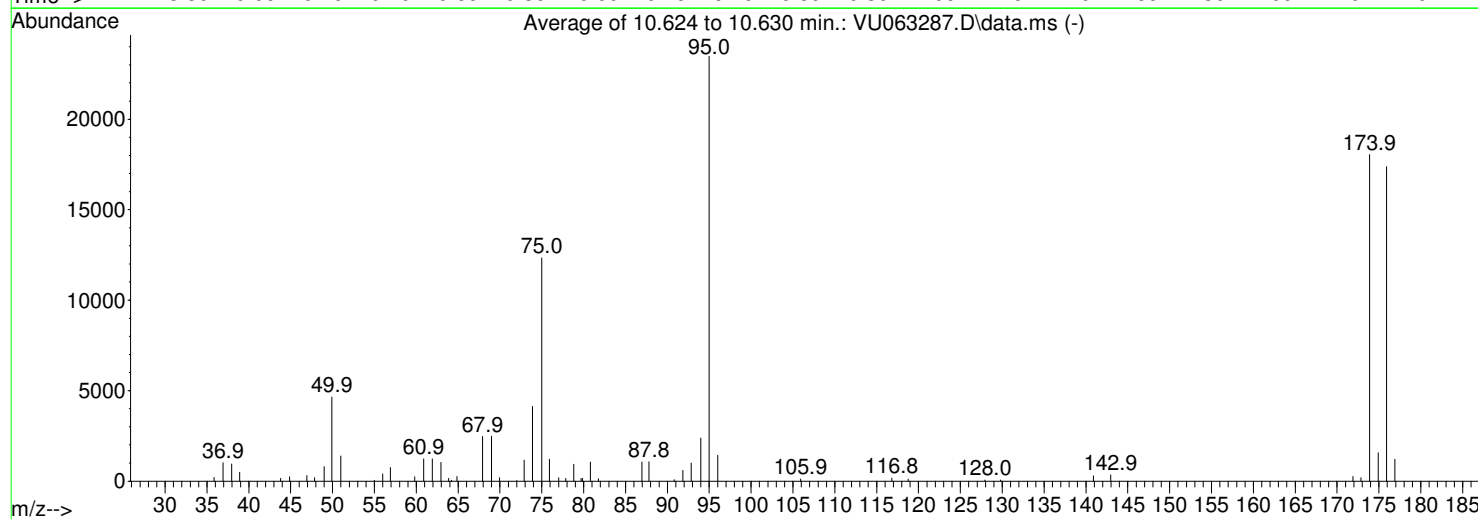


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031725\
Data File : VU063287.D
Acq On : 17 Mar 2025 09:35
Operator : MD/SY
Sample : BFB084
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB084

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031725WMA.M
Title : VOC Analysis
Last Update : Fri Mar 21 09:28:56 2025

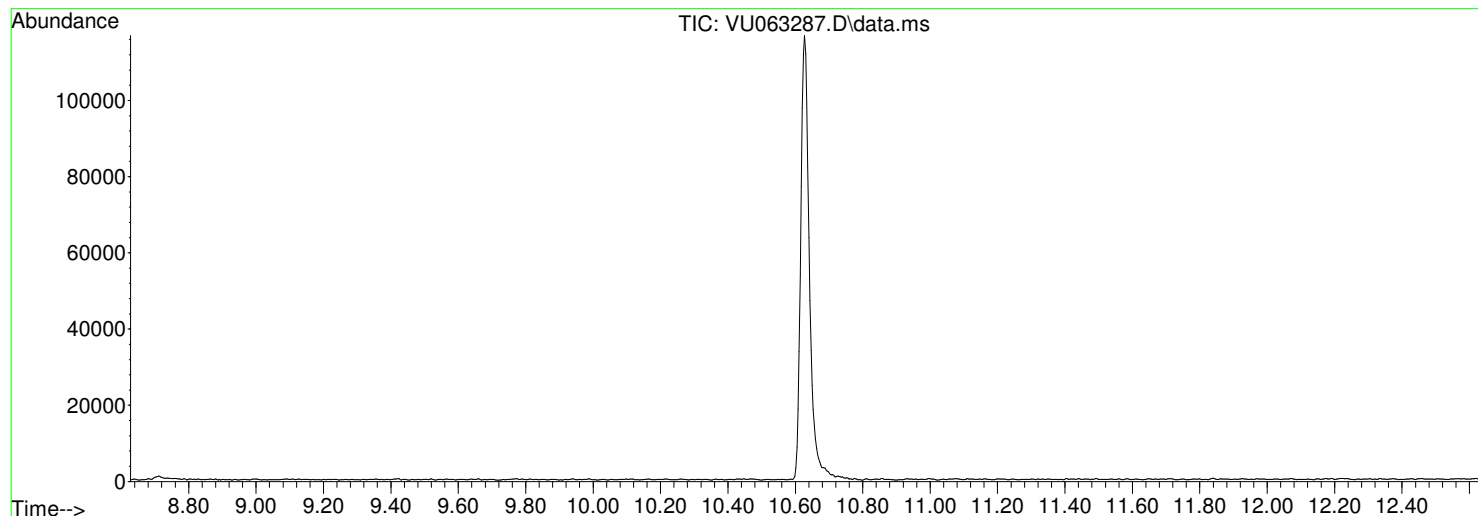

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	4634	PASS
75	95	30	80	52.5	12329	PASS
95	95	100	100	100.0	23477	PASS
96	95	5	9	6.1	1430	PASS
173	174	0.00	2	1.1	195	PASS
174	95	50	120	76.8	18040	PASS
175	174	5	9	8.7	1570	PASS
176	174	95	101	96.3	17379	PASS
177	176	5	9	7.0	1216	PASS

m/z	Abundance
39.90	273.0
43.80	273.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084

m/z	Abundance
35.80	214.0
36.90	982.0
38.00	936.0
38.90	502.0
39.90	211.0
43.90	412.0
44.90	194.0
46.90	314.0
47.90	201.0
49.00	730.0
49.90	4860.0
51.00	1337.0
56.00	417.0
56.90	768.0
59.80	245.0
60.90	1192.0
61.90	1362.0
62.90	963.0
63.80	138.0
64.20	153.0
64.90	262.0
67.90	2391.0
69.00	2365.0
70.00	192.0
72.00	100.0
72.90	1187.0
73.90	4029.0
75.00	12383.0
75.90	1249.0
77.00	148.0
77.80	145.0
78.80	944.0
79.70	204.0
79.90	204.0
80.80	1052.0
81.70	156.0
86.90	971.0
87.80	1082.0
90.80	145.0
91.90	593.0
92.90	1012.0
94.00	2363.0
95.00	23272.0
96.00	1402.0
105.90	124.0
116.80	137.0
118.70	102.0
140.90	262.0
142.90	311.0
171.90	239.0
172.90	220.0
173.90	17248.0
174.90	1476.0
175.90	17000.0
176.90	1284.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084

m/z	Abundance
35.80	184.0
36.90	1011.0
37.90	948.0
38.90	509.0
39.80	233.0
43.80	401.0
44.80	252.0
46.90	327.0
47.90	182.0
49.00	824.0
49.90	4731.0
51.00	1457.0
56.00	411.0
56.90	767.0
59.80	249.0
60.90	1277.0
61.90	1254.0
63.00	1067.0
63.80	161.0
64.80	266.0
67.90	2547.0
69.00	2516.0
70.00	188.0
72.90	1177.0
73.90	4297.0
75.00	12736.0
75.90	1287.0
77.00	201.0
77.80	148.0
78.80	971.0
79.70	225.0
80.80	1077.0
81.70	131.0
87.00	1062.0
87.80	1106.0
90.80	112.0
91.80	606.0
92.90	1010.0
94.00	2376.0
95.00	24296.0
96.00	1475.0
105.90	126.0
116.80	168.0
118.80	119.0
127.90	103.0
129.80	104.0
140.90	316.0
143.00	368.0
171.90	263.0
172.80	188.0
173.90	18536.0
174.90	1650.0
175.90	17824.0
176.90	1224.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084

m/z	Abundance
35.90	213.0
36.90	1039.0
37.90	929.0
38.90	440.0
39.80	242.0
43.90	457.0
44.80	281.0
47.00	288.0
47.80	170.0
49.00	846.0
49.90	4311.0
51.00	1373.0
55.00	113.0
56.00	349.0
56.90	724.0
59.80	242.0
60.90	1227.0
61.90	1079.0
62.90	1059.0
63.90	167.0
64.80	249.0
67.90	2442.0
69.00	2552.0
69.90	196.0
72.90	1117.0
73.90	4039.0
75.00	11869.0
75.90	1114.0
77.00	195.0
77.90	154.0
78.80	892.0
79.80	228.0
80.80	1026.0
81.80	127.0
87.00	1143.0
87.80	1000.0
91.80	559.0
92.80	996.0
94.00	2412.0
95.00	22864.0
96.00	1412.0
105.90	112.0
116.80	175.0
118.80	136.0
128.00	104.0
129.80	102.0
140.90	295.0
143.00	332.0
171.90	281.0
172.80	178.0
173.90	18336.0
174.90	1583.0
175.90	17312.0
176.90	1141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB084