

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031824\
 Data File : VU058145.D
 Acq On : 18 Mar 2024 12:58
 Operator : MD/SY
 Sample : P1779-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAKO

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU058145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.483	53	60	69	rBV	18279	18236	2.35%	0.396%
2	1.592	85	94	107	rVB	67504	75521	9.71%	1.638%
3	1.904	182	191	203	rVB	60140	77494	9.97%	1.681%
4	2.557	383	394	404	rBV	107367	175481	22.57%	3.807%
5	2.612	404	411	439	rVB	35552	66689	8.58%	1.447%
6	4.612	1019	1033	1048	rBV	54918	136279	17.53%	2.956%
7	4.692	1049	1058	1083	rVB	36872	94280	12.13%	2.045%
8	5.039	1152	1166	1197	rBV3	298827	777370	100.00%	16.864%
9	5.718	1358	1377	1402	rBV2	200858	510655	65.69%	11.078%
10	6.242	1524	1540	1560	rBV	160604	313923	40.38%	6.810%
11	6.682	1664	1677	1697	rBV2	118669	237276	30.52%	5.147%
12	7.560	1939	1950	1969	rBV	49545	90560	11.65%	1.965%
13	7.891	2041	2053	2071	rBV	231690	413060	53.14%	8.961%
14	8.177	2132	2142	2167	rBV2	26150	47722	6.14%	1.035%
15	8.628	2271	2282	2328	rBV2	183616	405260	52.13%	8.792%
16	9.412	2514	2526	2553	rBV	219822	381047	49.02%	8.266%
17	10.750	2931	2942	2962	rVB	69298	116412	14.98%	2.525%
18	10.888	2976	2985	2997	rVB3	6228	10315	1.33%	0.224%
19	11.807	3257	3271	3296	rBV	201990	336784	43.32%	7.306%
20	12.187	3377	3389	3418	rBV	189099	317149	40.80%	6.880%
21	12.769	3558	3570	3579	rVB	5344	8051	1.04%	0.175%




Sum of corrected areas: 4609564

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031824\
Data File : VU058145.D
Acq On : 18 Mar 2024 12:58
Operator : MD/SY
Sample : P1779-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COAK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

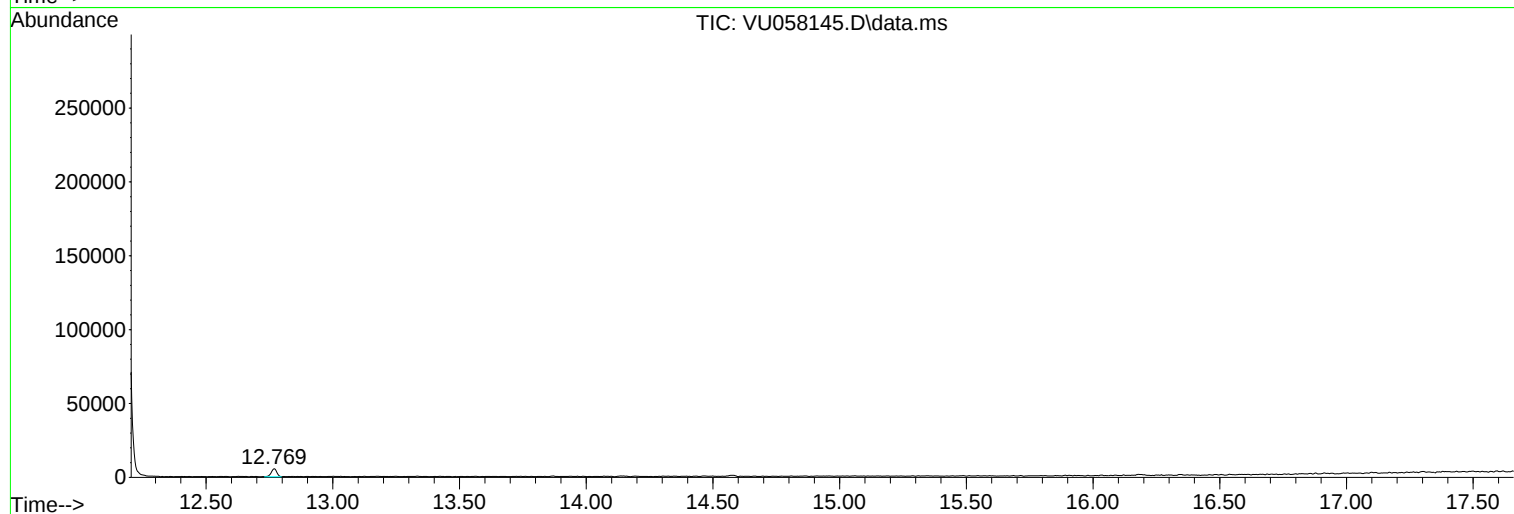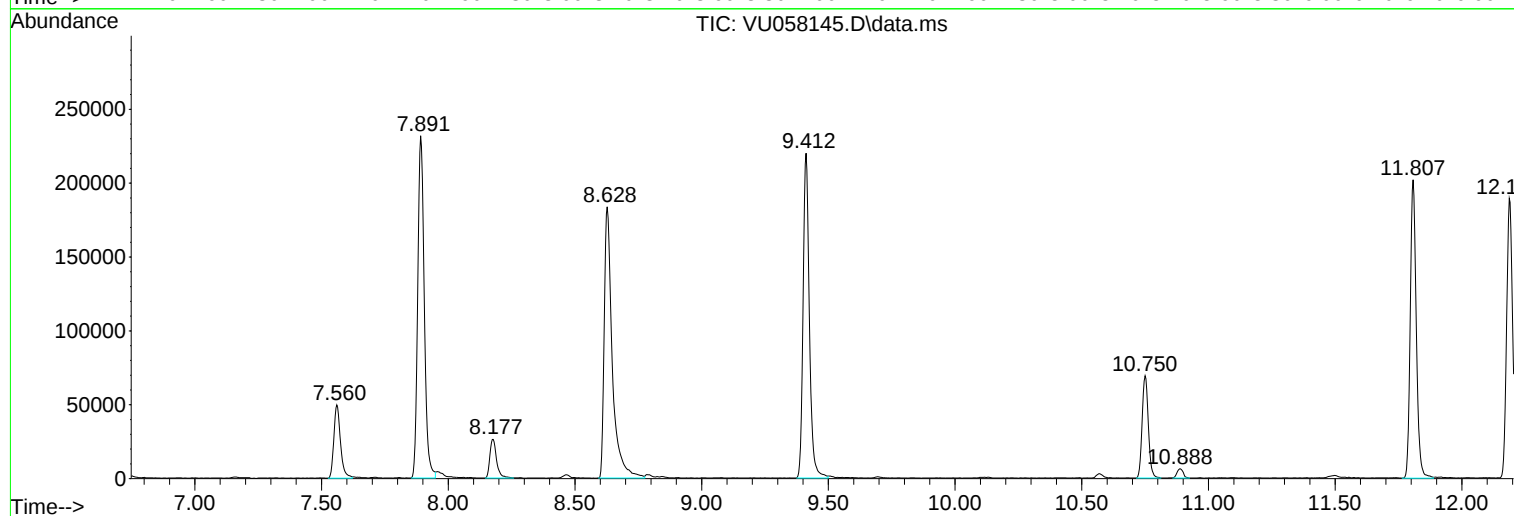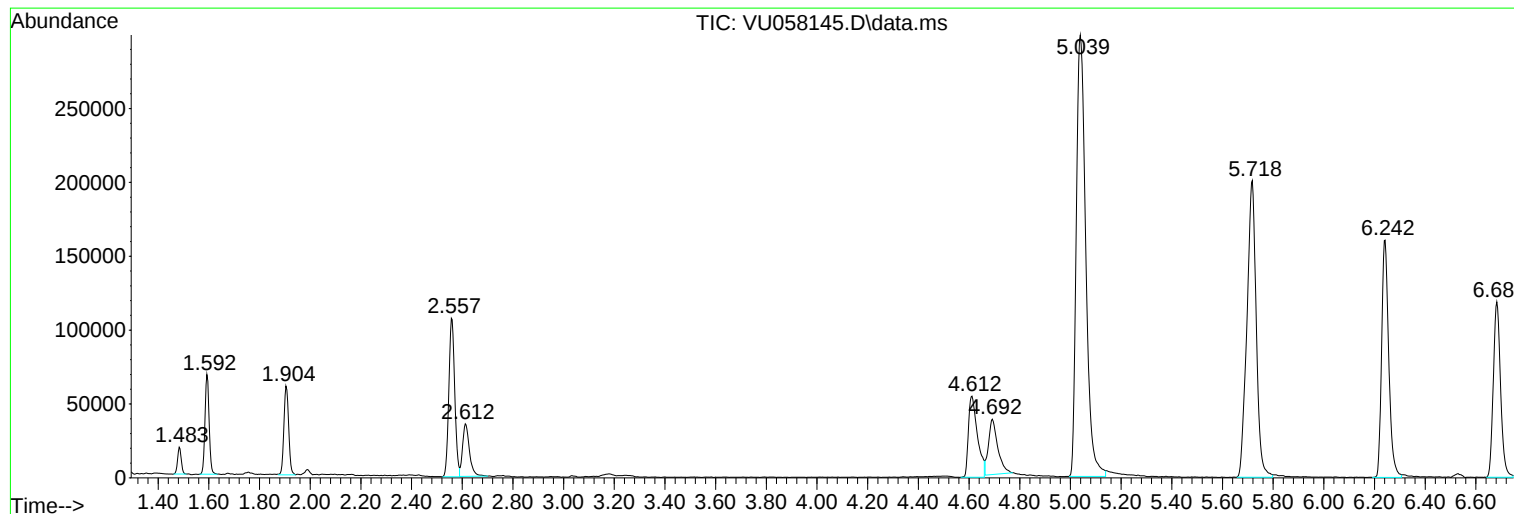

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031824\
Data File : VU058145.D
Acq On : 18 Mar 2024 12:58
Operator : MD/SY
Sample : P1779-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031824\
Data File : VU058145.D
Acq On : 18 Mar 2024 12:58
Operator : MD/SY
Sample : P1779-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc