


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031825\
Data File : VU063298.D
Acq On : 18 Mar 2025 10:43
Operator : MD/SY
Sample : BFB085
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB085

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031725WMA.M
Title : VOC Analysis
Last Update : Mon Mar 24 12:29:15 2025

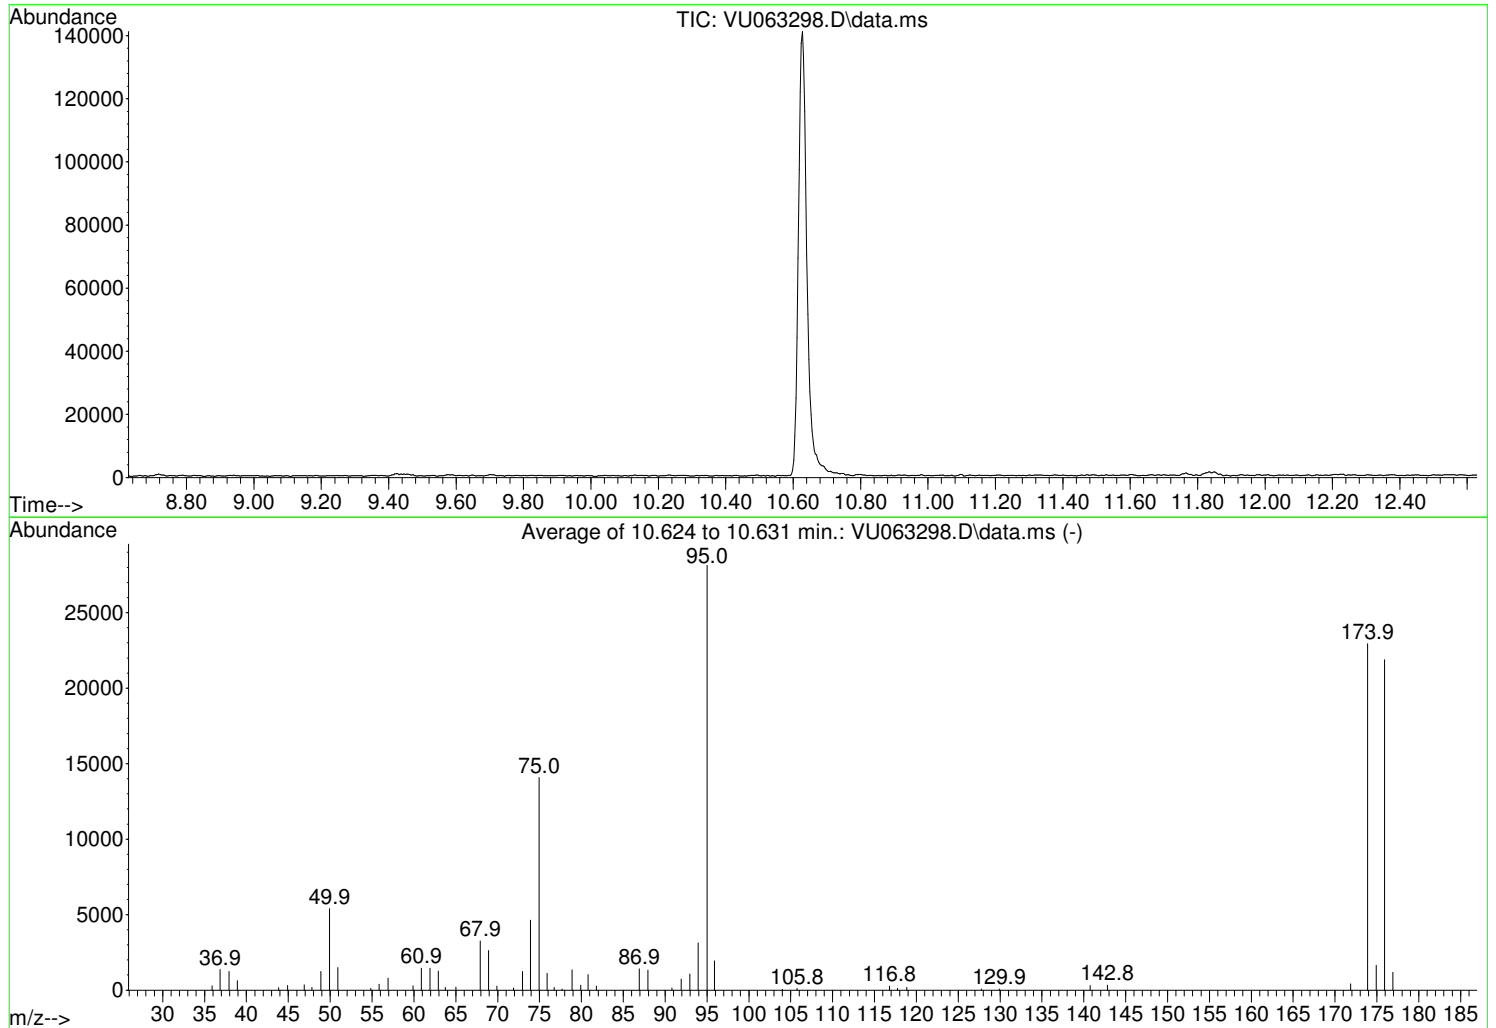

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	5397	PASS
75	95	30	80	50.0	14084	PASS
95	95	100	100	100.0	28141	PASS
96	95	5	9	6.9	1934	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.5	22947	PASS
175	174	5	9	7.2	1647	PASS
176	174	95	101	95.4	21888	PASS
177	176	5	9	5.4	1181	PASS

m/z	Abundance
39.80	255.0
43.80	432.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085

m/z	Abundance
35.90	269.0
36.90	1379.0
37.90	1253.0
38.90	643.0
39.80	212.0
43.90	617.0
44.90	318.0
46.90	436.0
47.80	148.0
48.90	1281.0
49.90	5395.0
50.90	1509.0
54.90	141.0
55.90	398.0
56.90	798.0
59.90	303.0
60.90	1465.0
61.90	1414.0
62.90	1239.0
63.80	178.0
65.00	184.0
67.90	3224.0
68.90	2659.0
69.90	284.0
71.90	181.0
73.00	1221.0
73.90	4933.0
75.00	14256.0
75.90	1103.0
76.80	143.0
77.70	129.0
78.90	1331.0
79.90	327.0
80.80	1003.0
81.80	324.0
86.90	1480.0
88.00	1309.0
90.80	109.0
91.90	726.0
92.90	1046.0
93.90	2920.0
95.00	28552.0
95.90	1930.0
104.00	152.0
105.80	120.0
116.80	228.0
117.70	122.0
118.80	196.0
129.90	117.0
140.70	306.0
142.80	320.0
171.80	348.0
173.90	22528.0
174.90	1676.0
175.90	21464.0
176.90	1167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085

m/z	Abundance
35.90	299.0
36.80	1397.0
37.90	1292.0
38.90	636.0
39.80	193.0
43.90	593.0
44.90	307.0
46.90	353.0
47.80	197.0
48.90	1261.0
49.90	5614.0
50.90	1514.0
54.90	123.0
55.90	402.0
56.90	789.0
59.90	294.0
60.90	1493.0
61.90	1462.0
62.90	1295.0
63.70	199.0
65.00	194.0
67.90	3349.0
68.90	2677.0
69.90	283.0
71.90	153.0
73.00	1253.0
73.90	4712.0
75.00	14369.0
75.90	1104.0
76.70	187.0
77.70	110.0
78.90	1390.0
79.90	354.0
80.80	1071.0
81.80	254.0
86.90	1446.0
87.90	1358.0
90.80	151.0
91.90	722.0
92.90	1105.0
94.00	3189.0
95.00	28944.0
95.90	2003.0
105.80	126.0
116.80	260.0
117.70	131.0
118.90	183.0
127.80	102.0
129.90	120.0
140.80	337.0
142.80	321.0
171.90	428.0
173.90	23624.0
174.90	1725.0
175.90	22680.0
176.90	1203.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085

m/z	Abundance
35.90	271.0
36.80	1300.0
37.90	1193.0
38.90	591.0
39.90	181.0
43.90	586.0
44.90	272.0
46.90	295.0
47.80	184.0
48.90	1191.0
49.90	5181.0
50.90	1437.0
54.80	100.0
55.80	395.0
56.90	767.0
59.90	241.0
60.90	1415.0
61.90	1503.0
62.90	1226.0
63.70	191.0
65.00	209.0
67.90	3161.0
68.90	2514.0
69.90	262.0
71.90	105.0
72.90	1220.0
73.90	4261.0
74.90	13627.0
75.90	1103.0
76.70	194.0
78.90	1310.0
79.90	322.0
80.80	995.0
81.80	212.0
86.90	1310.0
87.90	1313.0
90.80	156.0
91.90	736.0
93.00	1088.0
94.00	3297.0
95.00	26928.0
95.90	1869.0
105.70	105.0
116.80	304.0
117.80	116.0
118.90	161.0
127.70	111.0
140.80	306.0
142.80	328.0
171.90	462.0
173.90	22688.0
174.90	1540.0
175.90	21520.0
176.90	1174.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085