

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031925\
 Data File : VU063309.D
 Acq On : 19 Mar 2025 14:06
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK012

Quant Time: Mar 25 10:11:18 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM031925.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Mar 25 10:03:18 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	11411	0.50	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	15630	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	4686	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.590	65	3535	0.48	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	96.00%
4) 1,2-Dichloroethane-d4	5.685	65	2740	0.44	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	88.00%
7) 1,2-Dichloropropane-d6	6.687	67	2525	0.50	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	100.00%
8) Toluene-d8	7.887	98	6227	0.46	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	92.00%
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1991	0.46	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	92.00%
Target Compounds						
					Qvalue	
6) Trichloroethene	6.544	95	389	0.03	ug/L	93
12) 1,2,3-Trichloropropane	10.814	75	121	0.02	ug/L	88
13) 1,2-Dibromo-3-chloropr...	13.008	75	74	0.06	ug/L #	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031925\
Data File : VU063309.D
Acq On : 19 Mar 2025 14:06
Operator : MD/SY
Sample : VIBLK
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK012

Quant Time: Mar 25 10:11:18 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM031925.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Mar 25 10:03:18 2025
Response via : Initial Calibration

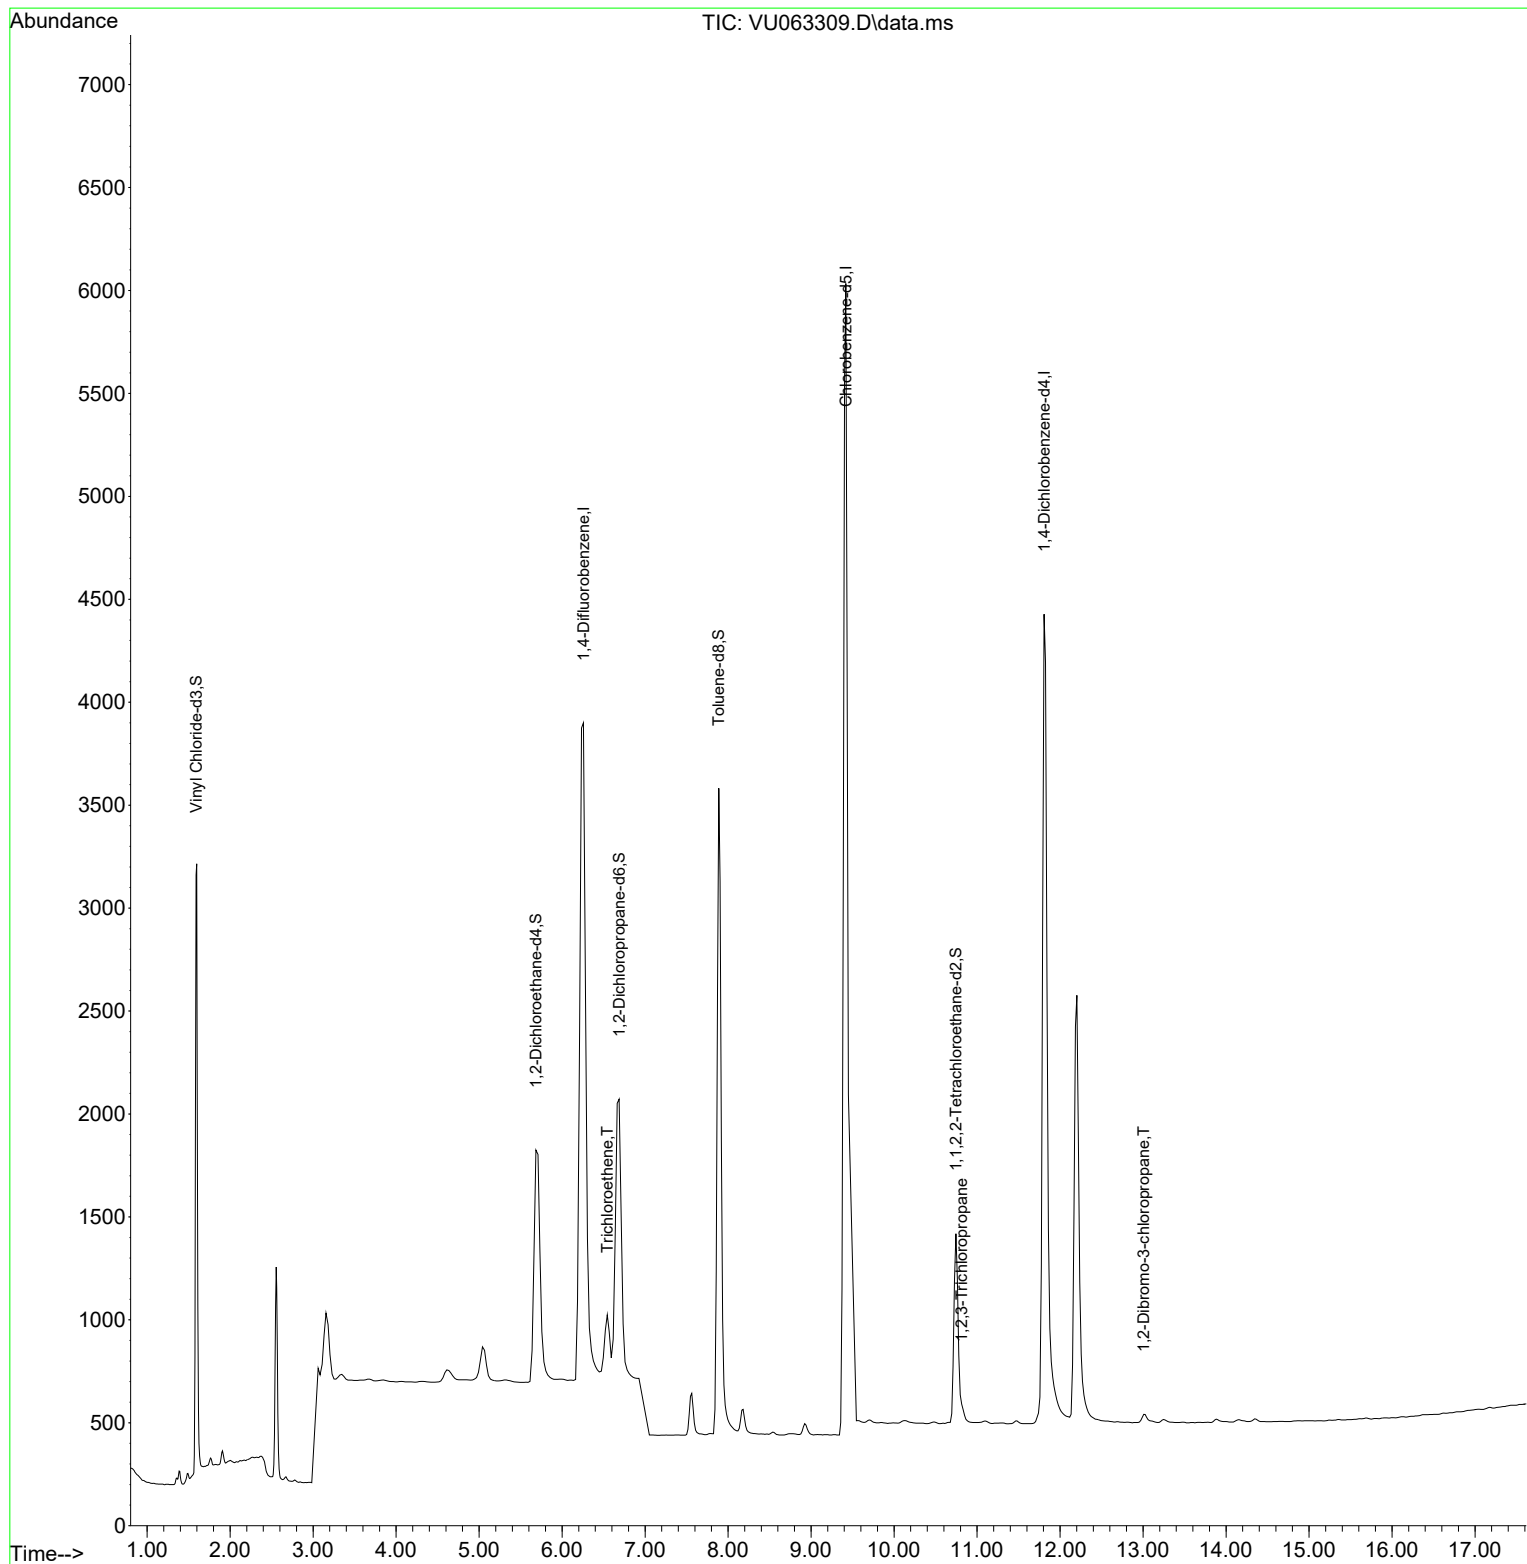

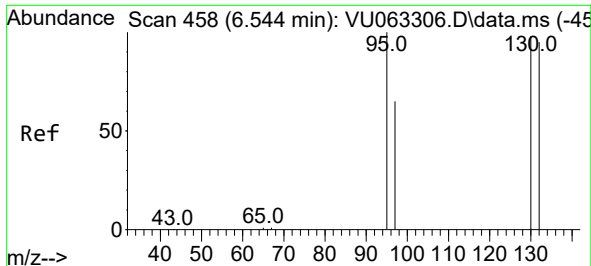

#6
Trichloroethene

Concen: 0.03 ug/L

RT: 6.544 min Scan# 458

Delta R.T. 0.000 min

Lab File: VU063309.D

Acq: 19 Mar 2025 14:06

Instrument :

MSVOA_U

ClientSampleId :

VIBLK012

Tgt Ion: 95 Resp: 389





Ion Ratio Lower Upper

95 100

97 80.3 46.6 86.6

132 90.9 66.7 123.9

130 99.2 68.6 127.4

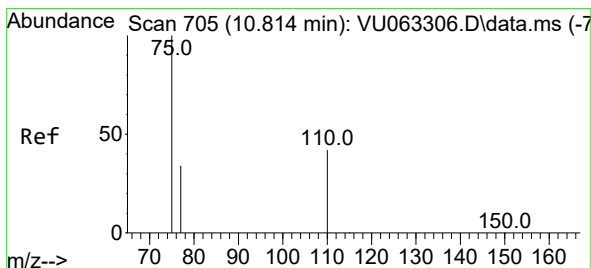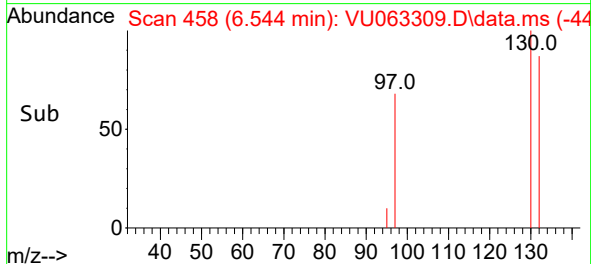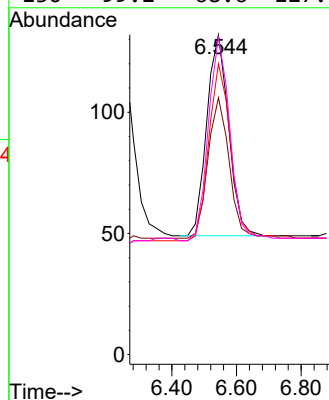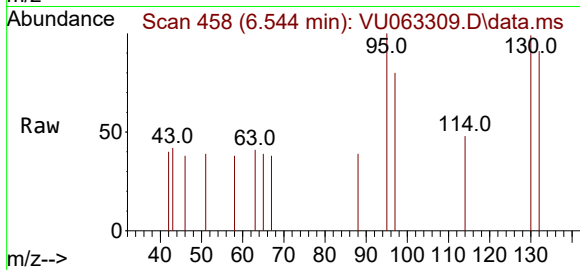

#12

1,2,3-Trichloropropane

Concen: 0.02 ug/L

RT: 10.814 min Scan# 705

Delta R.T. -0.000 min

Lab File: VU063309.D

Acq: 19 Mar 2025 14:06




Tgt Ion: 75 Resp: 121


Ion Ratio Lower Upper

75 100

110 33.1 32.7 49.1

77 40.5 27.1 40.7

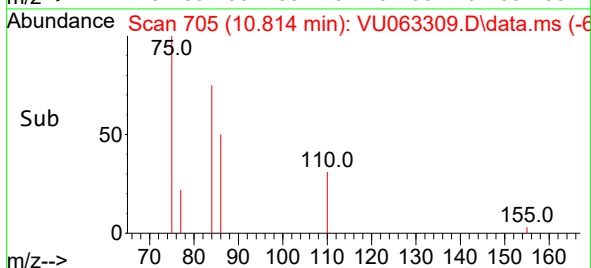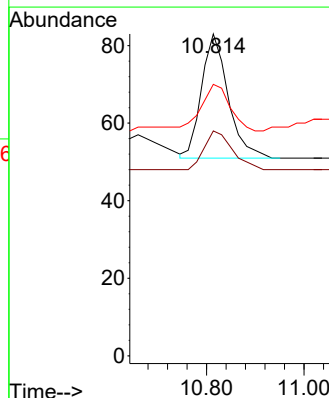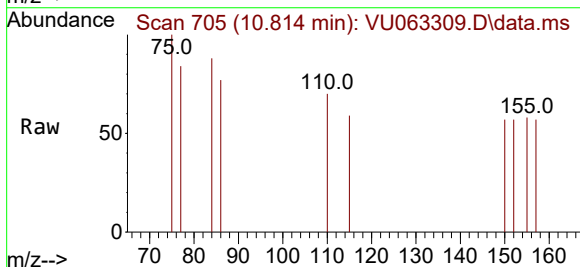

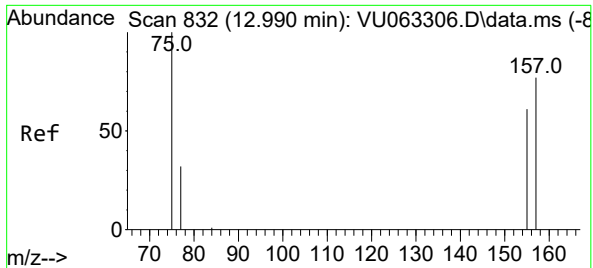

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.06 ug/L
 RT: 13.008 min Scan# 81
 Delta R.T. 0.018 min
 Lab File: VU063309.D
 Acq: 19 Mar 2025 14:06

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK012

Tgt Ion: 75	Resp:	74
Ion Ratio	Lower	Upper
75	100	
157	90.8	65.4 98.2
155	87.7	55.8 83.6#

