


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032124\
Data File : VU058178.D
Acq On : 21 Mar 2024 09:29
Operator : MD/SY
Sample : BFB127
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB127

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Mar 22 04:55:54 2024

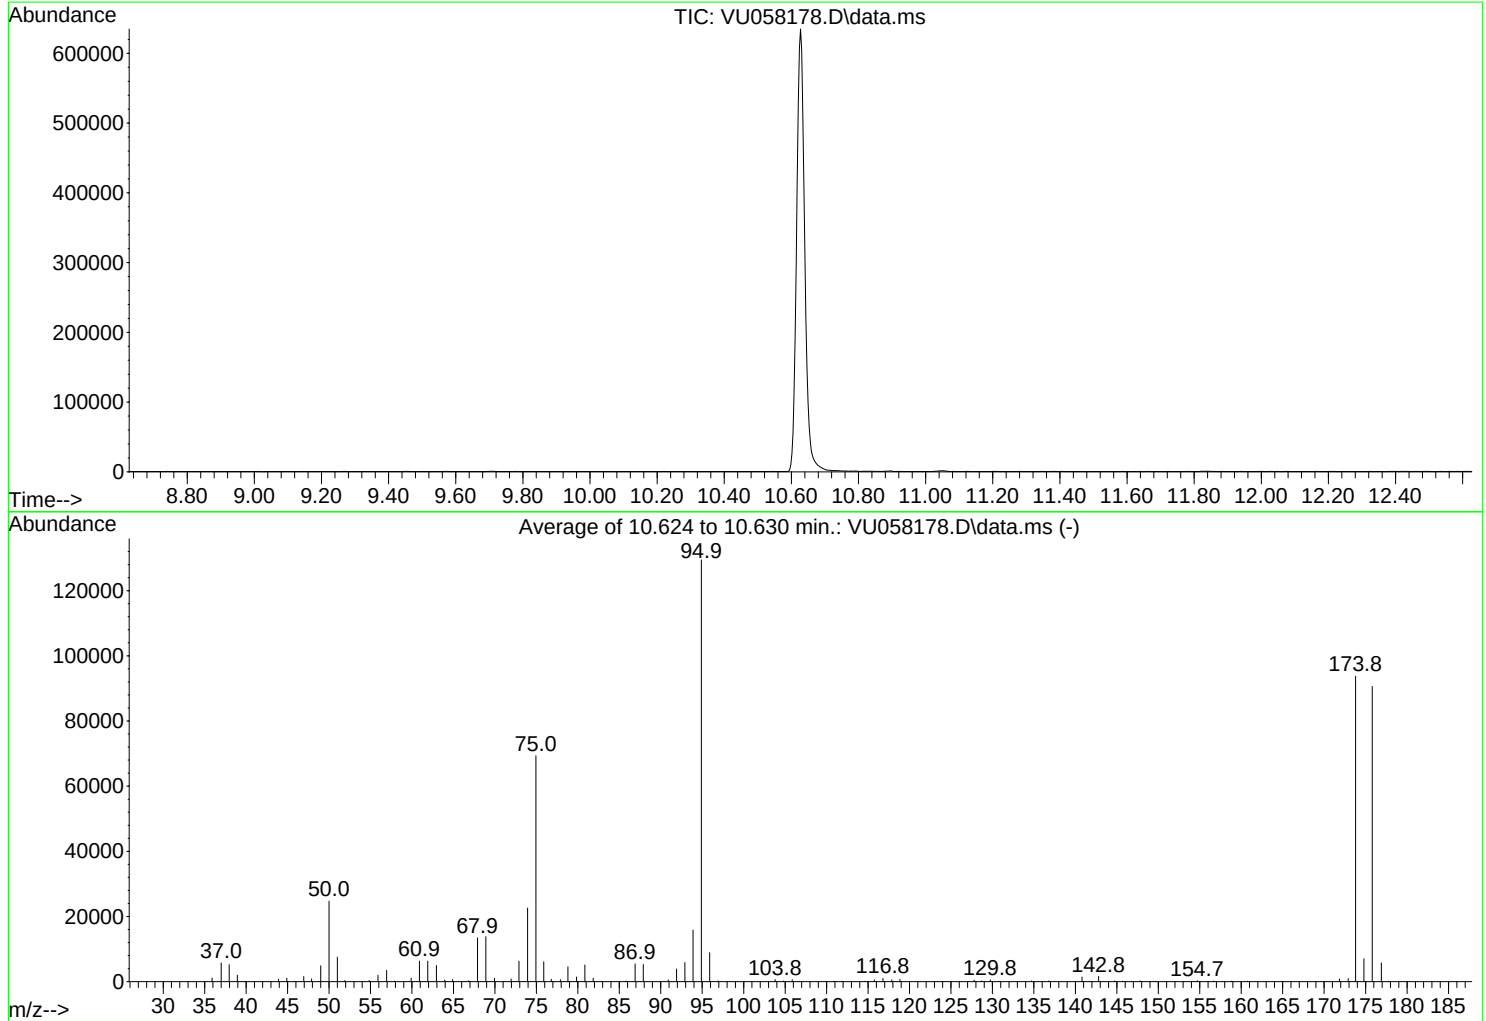

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	24720	PASS
75	95	30	80	53.6	69371	PASS
95	95	100	100	100.0	129464	PASS
96	95	5	9	6.9	8892	PASS
173	174	0.00	2	1.0	933	PASS
174	95	50	120	72.4	93757	PASS
175	174	5	9	7.5	7001	PASS
176	174	95	101	96.7	90624	PASS
177	176	5	9	6.4	5759	PASS

m/z	Abundance
39.80	176.0
43.90	244.0

Instrument :
MSVOA_U
ClientSampleId :
BFB127

m/z	Abundance
35.90	1050.0
37.00	5635.0
37.90	5113.0
39.00	2014.0
39.90	263.0
43.90	891.0
44.90	1089.0
45.90	148.0
47.00	1692.0
47.90	846.0
49.00	4861.0
50.00	24648.0
51.00	7682.0
51.90	318.0
54.80	428.0
55.90	2064.0
56.90	3518.0
57.90	238.0
59.90	1064.0
60.90	6401.0
61.90	6495.0
62.90	4872.0
63.90	494.0
64.90	652.0
66.80	296.0
67.90	13457.0
68.90	13739.0
69.90	1064.0
72.00	816.0
72.90	6376.0
74.00	22424.0
75.00	68848.0
75.90	5951.0
76.80	663.0
77.90	566.0
78.80	4523.0
79.80	1471.0
80.80	5178.0
81.80	1111.0
82.90	131.0
85.80	192.0
86.90	5319.0
87.90	5455.0
90.90	546.0
91.90	3843.0
92.90	5690.0
93.90	15842.0
94.90	128200.0
95.90	8974.0
96.90	231.0
103.80	581.0
104.80	179.0
105.90	640.0
106.80	142.0
110.80	115.0
111.80	115.0
114.90	161.0
115.80	586.0
116.80	969.0
117.90	525.0
118.90	724.0
127.80	460.0
128.70	225.0
129.80	531.0
130.90	143.0
134.70	255.0
136.80	231.0
140.80	1373.0
141.70	128.0
142.80	1601.0
144.80	267.0
145.70	131.0
146.80	133.0
147.90	263.0
148.90	110.0
154.70	296.0
156.70	237.0
158.90	137.0
160.70	144.0
171.90	696.0
172.90	935.0
173.80	90432.0
174.80	6756.0
175.80	88432.0
176.90	5729.0
177.80	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB127

m/z	Abundance
35.90	1118.0
37.00	5946.0
37.90	5412.0
38.90	2010.0
39.90	260.0
43.90	953.0
44.90	1116.0
45.80	132.0
47.00	1609.0
47.90	856.0
49.00	4967.0
50.00	25448.0
51.00	7765.0
51.90	371.0
54.90	415.0
55.90	2029.0
57.00	3547.0
57.90	205.0
59.90	1088.0
60.90	6466.0
61.90	6464.0
63.00	5055.0
64.00	491.0
64.90	661.0
66.80	307.0
67.90	13810.0
68.90	14193.0
69.90	1051.0
72.00	905.0
72.90	6532.0
74.00	23216.0
75.00	71656.0
75.90	6336.0
76.80	748.0
77.90	633.0
78.80	4743.0
79.80	1491.0
80.80	5232.0
81.90	1113.0
82.80	108.0
85.80	192.0
86.90	5705.0
87.90	5465.0
90.90	572.0
91.90	3977.0
92.90	5967.0
93.90	16340.0
94.90	133312.0
95.90	9213.0
96.90	269.0
103.80	673.0
104.80	205.0
105.90	617.0
106.70	115.0
110.80	148.0
111.90	136.0
114.60	142.0
115.00	128.0
115.80	559.0
116.80	1051.0
117.90	553.0
118.80	682.0
123.90	106.0
127.80	434.0
128.70	263.0
129.80	574.0
130.90	168.0
134.70	277.0
136.80	250.0
140.80	1539.0
141.80	122.0
142.80	1647.0
144.80	246.0
145.70	170.0
146.80	113.0
147.80	281.0
148.90	104.0
149.70	107.0
154.70	332.0
156.70	239.0
158.80	156.0
160.70	149.0
171.80	830.0
172.90	958.0
173.80	96432.0
174.80	7258.0
175.80	93432.0
176.90	6012.0
177.80	173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB127

m/z	Abundance
35.90	1046.0
37.00	5649.0
38.00	5099.0
38.90	1856.0
39.90	266.0
43.90	999.0
44.90	1006.0
46.90	1462.0
47.90	769.0
49.00	4730.0
50.00	24064.0
51.00	7171.0
51.90	401.0
54.90	367.0
55.90	1878.0
57.00	3306.0
57.90	125.0
59.90	1116.0
60.90	6009.0
61.90	5895.0
63.00	5008.0
64.00	488.0
64.90	596.0
66.90	307.0
67.90	13083.0
68.90	13426.0
70.00	1002.0
71.90	848.0
72.90	6004.0
73.90	22224.0
74.90	67608.0
75.90	5981.0
76.80	785.0
77.90	561.0
78.80	4436.0
79.90	1336.0
80.90	4867.0
81.80	1046.0
85.80	173.0
86.90	5328.0
87.90	4838.0
90.90	525.0
91.90	3782.0
92.90	5851.0
93.90	15235.0
94.90	126880.0
95.90	8490.0
96.90	302.0
103.80	744.0
104.80	229.0
105.80	586.0
110.90	180.0
111.90	150.0
114.60	122.0
115.70	553.0
116.80	1003.0
117.80	544.0
118.80	643.0
123.90	106.0
127.80	404.0
128.70	252.0
129.70	525.0
130.90	176.0
134.70	273.0
136.80	246.0
140.80	1437.0
141.80	125.0
142.80	1580.0
144.70	203.0
145.70	190.0
147.70	257.0
149.60	100.0
154.70	314.0
156.70	190.0
158.80	142.0
160.80	139.0
171.80	882.0
172.90	907.0
173.80	94408.0
174.80	6989.0
175.80	90008.0
176.90	5537.0
177.80	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB127