

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047718.D
 Acq On : 26 Mar 2022 18:44
 Operator : SY/MD
 Sample : N2081-20DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1


Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y7DL

Quant Time: Mar 28 05:11:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 28 05:05:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	315066	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	323472	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	173325	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	93919	41.107	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	82.220%		
7) Chloroethane-d5	1.915	69	89262	49.548	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	99.100%		
11) 1,1-Dichloroethene-d2	2.571	63	145921	34.908	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.820%		
21) 2-Butanone-d5	4.632	46	219403	111.880	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	111.880%		
24) Chloroform-d	5.066	84	196539	47.013	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.020%		
26) 1,2-Dichloroethane-d4	5.703	65	131506	51.290	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.580%		
32) Benzene-d6	5.729	84	395779	48.625	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.240%		
36) 1,2-Dichloropropane-d6	6.690	67	128286	51.321	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	102.640%		
41) Toluene-d8	7.899	98	361129	45.538	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.080%		
43) trans-1,3-Dichloroprop...	8.179	79	59129	46.691	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.380%		
47) 2-Hexanone-d5	8.635	63	162116	110.786	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	110.790%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	210899	49.161	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.320%		
66) 1,2-Dichlorobenzene-d4	12.195	152	158277	51.328	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.660%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.571	101	1422	0.612	ug/L #	18
12) 1,1-Dichloroethene	2.584	96	27332	12.647	ug/L #	37
19) 1,1-Dichloroethane	3.874	63	71954	17.898	ug/L	98
20) cis-1,2-Dichloroethene	4.671	96	22240	8.702	ug/L	96
30) 1,1,1-Trichloroethane	5.321	97	165057	45.001	ug/L	99
31) Carbon tetrachloride	5.321	117	22690	6.851	ug/L	99
34) Trichloroethene	6.546	95	16303	6.642	ug/L	97
39) cis-1,3-Dichloropropene	7.568	75	3635	0.984	ug/L #	49
44) trans-1,3-Dichloropropene	8.182	75	2684	0.728	ug/L #	75
46) Tetrachloroethene	8.555	164	18862	8.551	ug/L	98
49) Dibromochloromethane	8.555	129	16697	5.711	ug/L #	11





(#) = qualifier out of range (m) = manual integration (+) = signals summed

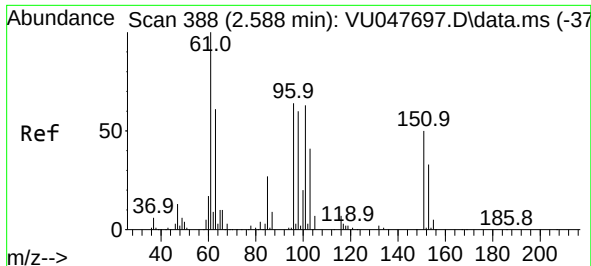

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.612 ug/L
 RT: 2.571 min Scan# 383
 Delta R.T. -0.016 min
 Lab File: VU047718.D
 Acq: 26 Mar 2022 18:44




Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y7DL


Tgt Ion:101 Resp: 1422
 Ion Ratio Lower Upper
 101 100
 85 0.0 32.8 49.2#
 151 0.0 63.0 94.6#

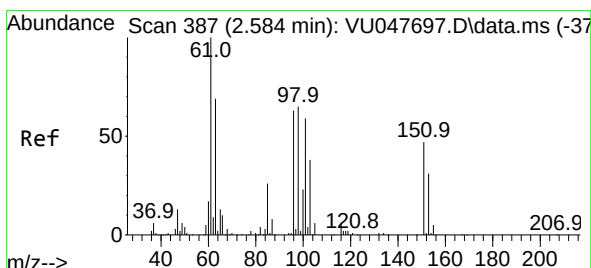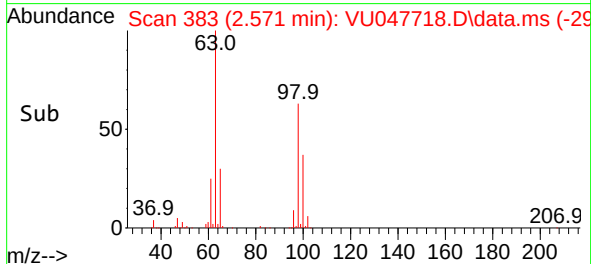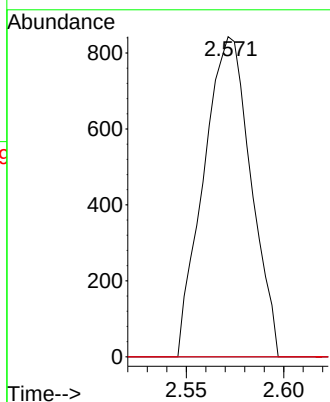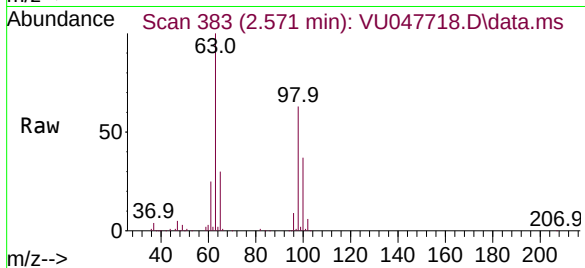

#12
 1,1-Dichloroethene
 Concen: 12.647 ug/L
 RT: 2.584 min Scan# 387
 Delta R.T. -0.000 min
 Lab File: VU047718.D
 Acq: 26 Mar 2022 18:44

Tgt Ion: 96 Resp: 27332
 Ion Ratio Lower Upper
 96 100
 61 180.0 113.1 210.1
 63 281.9 94.8 176.0#

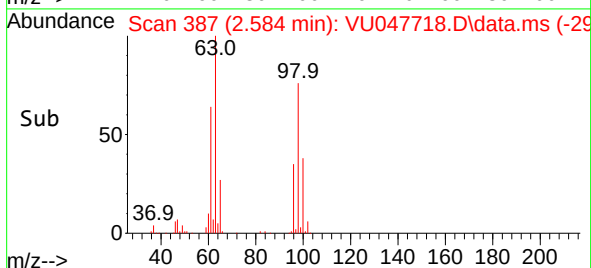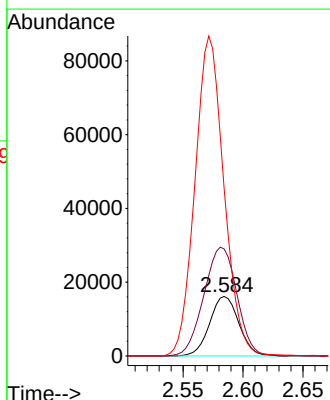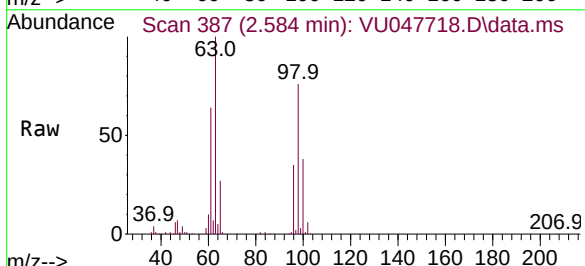

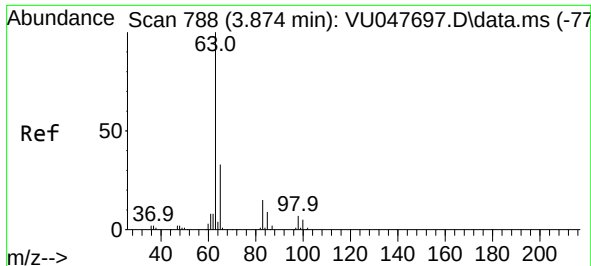

#19

1,1-Dichloroethane

Concen: 17.898 ug/L

RT: 3.874 min Scan# 719

Delta R.T. -0.000 min

Lab File: VU047718.D

Acq: 26 Mar 2022 18:44

Instrument :

MSVOA_U

ClientSampleId :

EW5Y7DL





Tgt Ion: 63 Resp: 71954

Ion Ratio Lower Upper

63 100

65 30.3 22.0 41.0

83 14.3 9.7 18.1

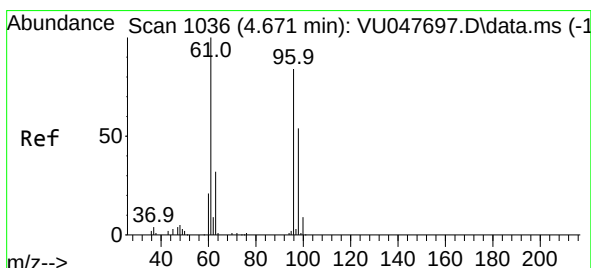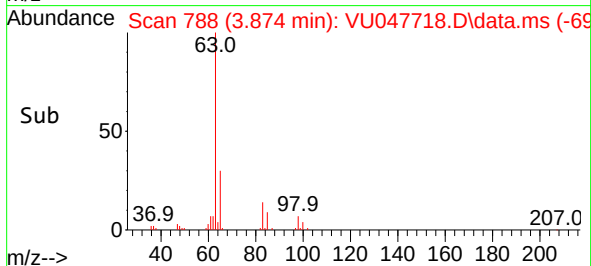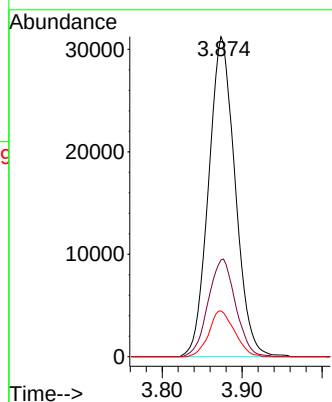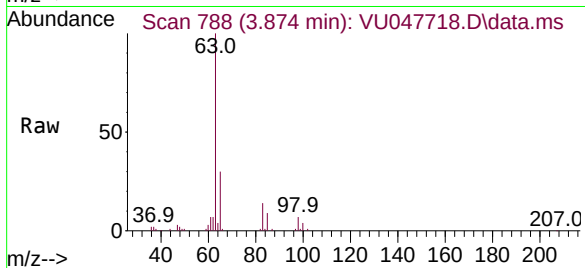

#20

cis-1,2-Dichloroethene

Concen: 8.702 ug/L

RT: 4.671 min Scan# 1036

Delta R.T. -0.000 min

Lab File: VU047718.D

Acq: 26 Mar 2022 18:44




Tgt Ion: 96 Resp: 22240


Ion Ratio Lower Upper

96 100

61 110.5 80.7 149.9

68 0.0 0.0 0.0

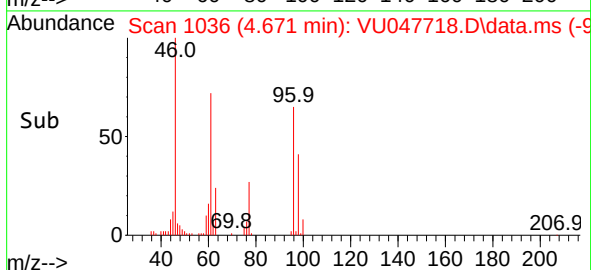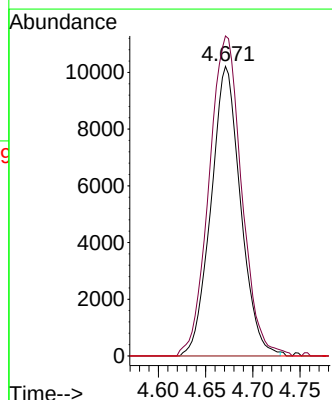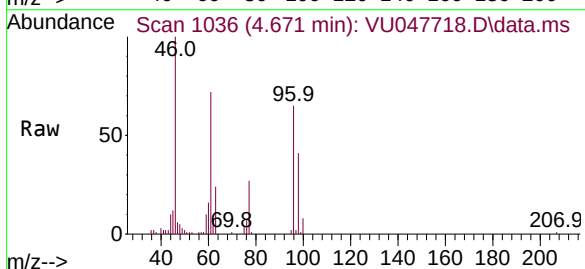

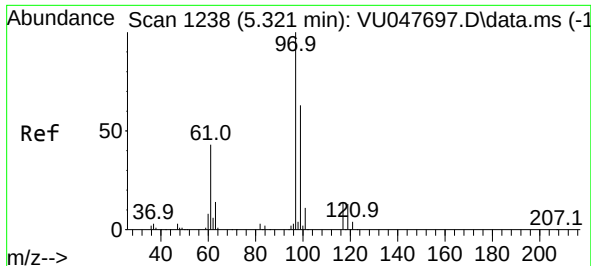

#30

1,1,1-Trichloroethane

Concen: 45.001 ug/L

RT: 5.321 min Scan# 1238

Delta R.T. -0.000 min

Lab File: VU047718.D

Acq: 26 Mar 2022 18:44

Instrument :

MSVOA_U

ClientSampleId :

EW5Y7DL





Tgt Ion: 97 Resp: 165057

Ion Ratio Lower Upper

97 100

99 64.9 51.6 77.4

61 44.6 34.2 51.4

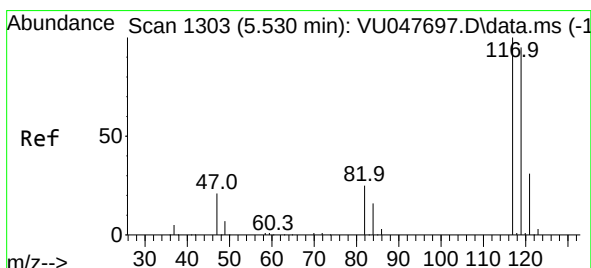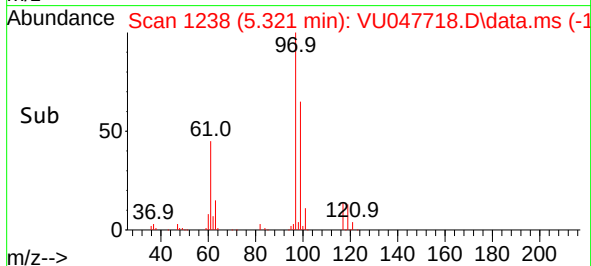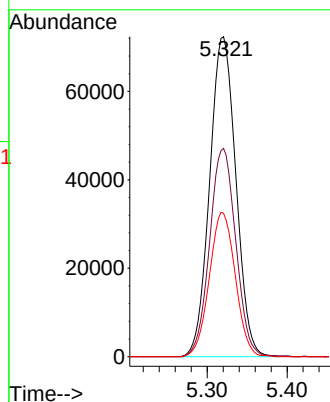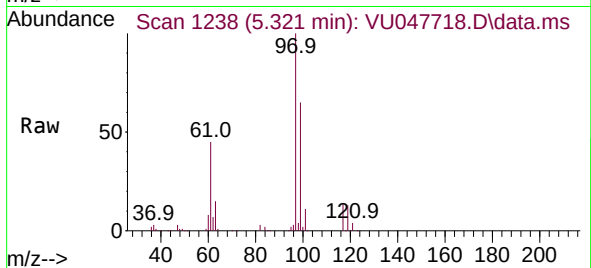

#31

Carbon tetrachloride

Concen: 6.851 ug/L

RT: 5.321 min Scan# 1238

Delta R.T. -0.209 min

Lab File: VU047718.D




Acq: 26 Mar 2022 18:44


Tgt Ion: 117 Resp: 22690

Ion Ratio Lower Upper

117 100

119 97.5 77.2 115.8


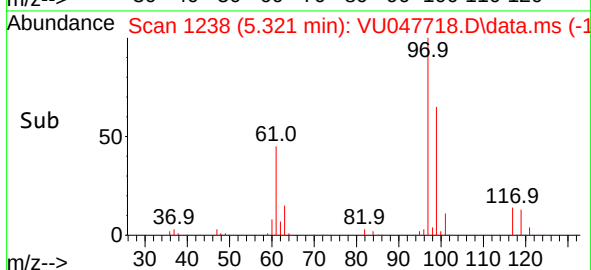
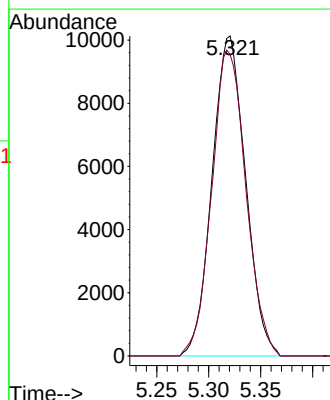
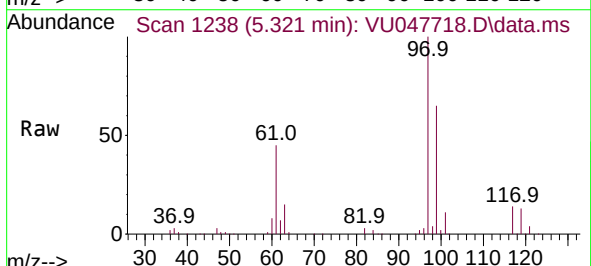


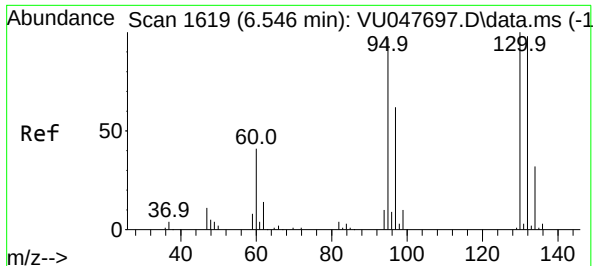

#34
Trichloroethene
Concen: 6.642 ug/L
RT: 6.546 min Scan# 1
Delta R.T. -0.000 min
Lab File: VU047718.D
Acq: 26 Mar 2022 18:44




Instrument :
MSVOA_U
ClientSampleId :
EW5Y7DL


Tgt Ion: 95 Resp: 16303
Ion Ratio Lower Upper
95 100
97 67.0 44.7 82.9
132 99.1 70.4 130.8
130 102.4 73.6 136.8

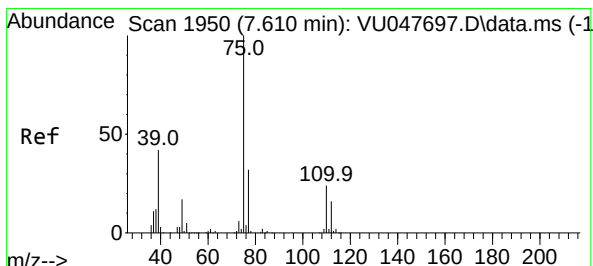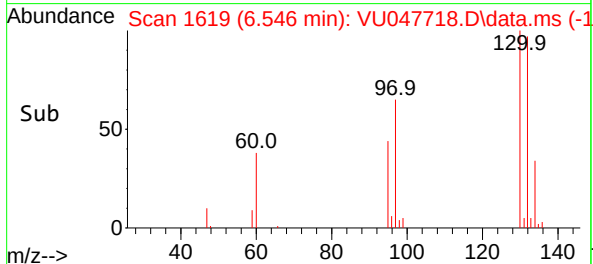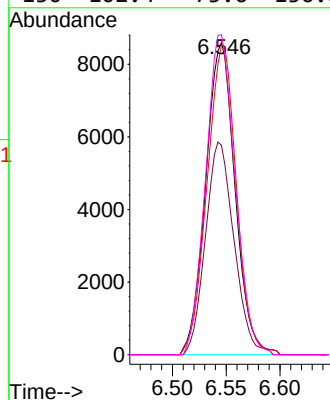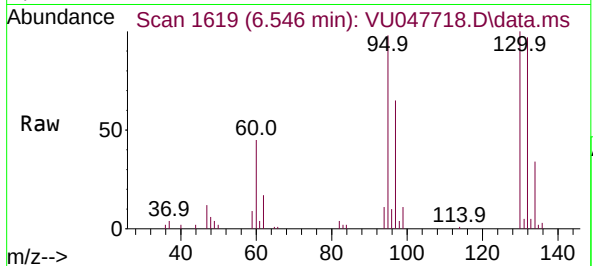

#39
cis-1,3-Dichloropropene
Concen: 0.984 ug/L
RT: 7.568 min Scan# 1937
Delta R.T. -0.042 min
Lab File: VU047718.D
Acq: 26 Mar 2022 18:44

Tgt Ion: 75 Resp: 3635
Ion Ratio Lower Upper
75 100
77 59.4 21.8 40.6#


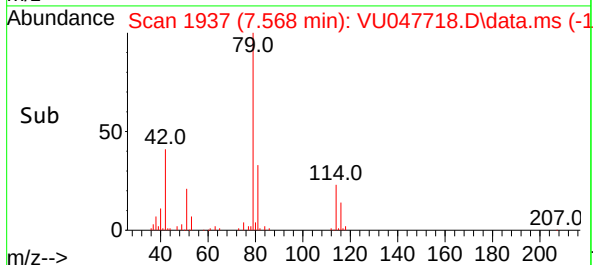
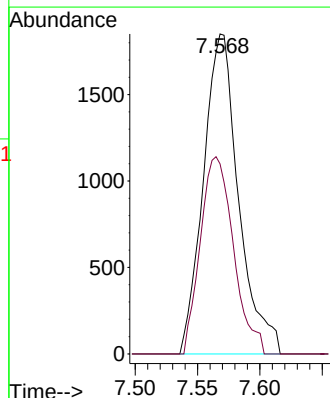
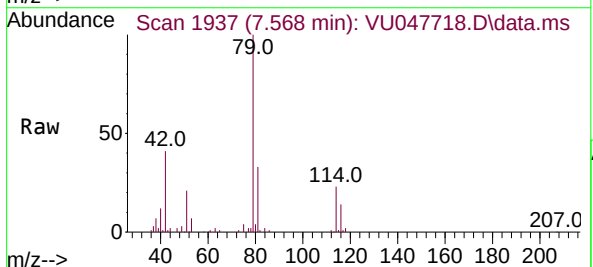


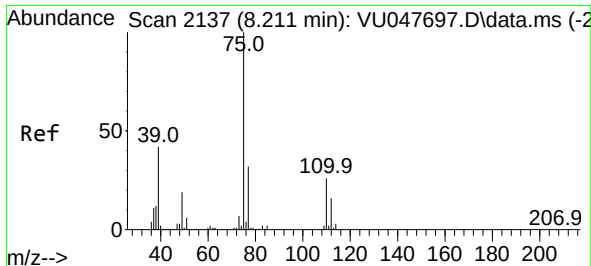

#44
trans-1,3-Dichloropropene
Concen: 0.728 ug/L
RT: 8.182 min Scan# 2137
Delta R.T. -0.029 min
Lab File: VU047718.D
Acq: 26 Mar 2022 18:44




Instrument :
MSVOA_U
ClientSampleId :
EW5Y7DL


Tgt Ion: 75 Resp: 2684
Ion Ratio Lower Upper
75 100
77 45.5 22.0 40.8#

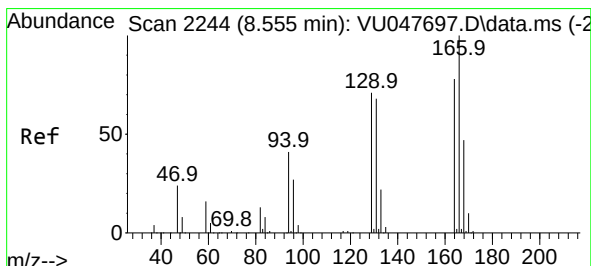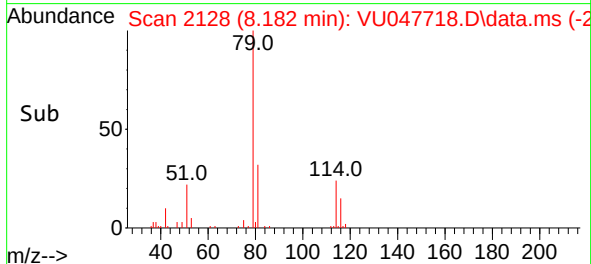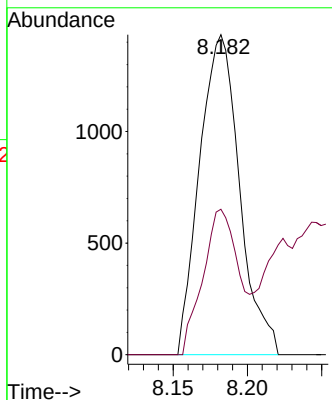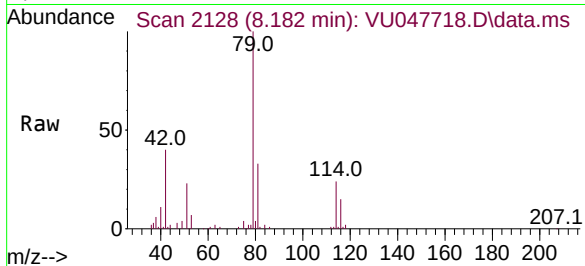

#46
Tetrachloroethene
Concen: 8.551 ug/L
RT: 8.555 min Scan# 2244
Delta R.T. -0.000 min
Lab File: VU047718.D
Acq: 26 Mar 2022 18:44

Tgt Ion:164 Resp: 18862
Ion Ratio Lower Upper
164 100
129 90.8 62.4 116.0
131 89.1 60.7 112.7
166 128.7 89.0 165.4

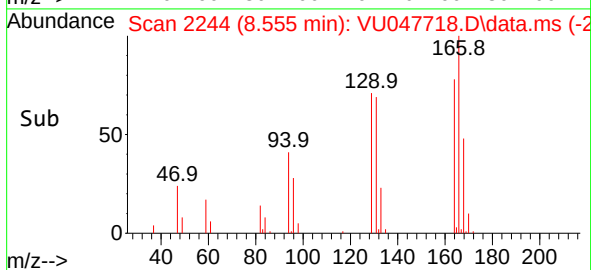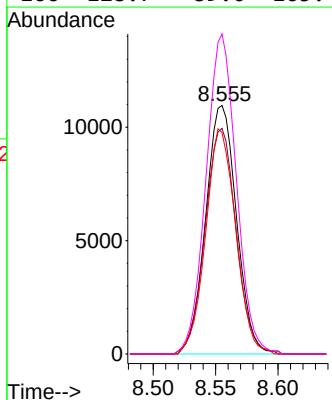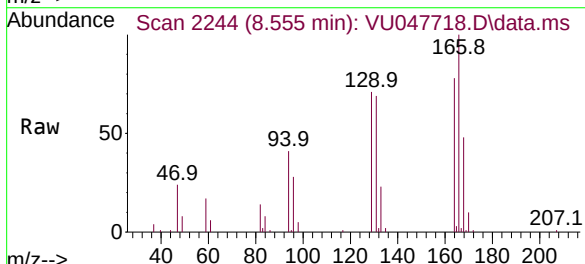

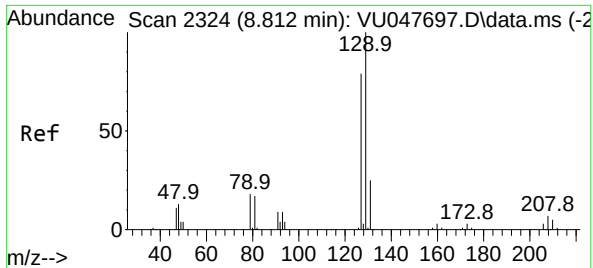

#49

Dibromochloromethane

Concen: 5.711 ug/L

RT: 8.555 min Scan# 21

Delta R.T. -0.257 min

Lab File: VU047718.D


Acq: 26 Mar 2022 18:44

Instrument :

MSVOA_U

ClientSampleId :

EW5Y7DL

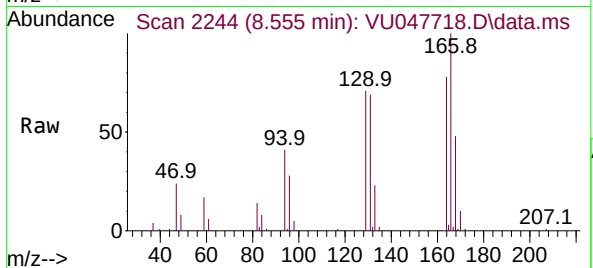

Tgt Ion:129 Resp: 16697

Ion Ratio Lower Upper

129 100

127 0.0 54.2 100.6#

