

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047698.D
 Acq On : 26 Mar 2022 10:55
 Operator : SY/MD
 Sample : VU0326WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK073

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047698.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	99	rBV	150882	176847	13.27%	1.599%
2	1.919	171	180	202	rBV	126472	175262	13.15%	1.584%
3	2.292	293	296	298	rBV2	867	628	0.05%	0.006%
4	2.572	370	383	410	rBV	269635	457042	34.30%	4.131%
5	2.797	449	453	456	rBV2	638	593	0.04%	0.005%
6	2.951	499	501	504	rVV3	302	231	0.02%	0.002%
7	3.054	524	533	544	rVB4	2201	4312	0.32%	0.039%
8	3.163	564	567	569	rBV	283	187	0.01%	0.002%
9	3.218	579	584	586	rBV2	222	201	0.02%	0.002%
10	3.234	586	589	594	rVB2	303	304	0.02%	0.003%
11	3.263	594	598	601	rBV2	233	203	0.02%	0.002%
12	3.359	623	628	629	rBV	395	334	0.03%	0.003%
13	3.510	668	675	677	rBV2	268	359	0.03%	0.003%
14	3.594	698	701	703	rVV	296	180	0.01%	0.002%
15	3.607	703	705	712	rVB2	316	382	0.03%	0.003%
16	3.639	712	715	719	rBV	218	213	0.02%	0.002%
17	3.665	719	723	727	rVB2	260	263	0.02%	0.002%
18	3.813	763	769	774	rVB2	239	203	0.02%	0.002%
19	3.903	793	797	800	rVV	242	192	0.01%	0.002%
20	3.951	810	812	816	rVB	271	209	0.02%	0.002%
21	4.092	852	856	860	rBV2	235	227	0.02%	0.002%
22	4.163	872	878	883	rBV2	211	253	0.02%	0.002%
23	4.346	932	935	941	rVB2	218	249	0.02%	0.002%
24	4.533	989	993	998	rVB2	281	304	0.02%	0.003%
25	4.639	1009	1026	1063	rBV	137349	421566	31.64%	3.811%
26	4.954	1117	1124	1134	rBV3	378	720	0.05%	0.007%
27	5.067	1143	1159	1190	rBV	241155	530316	39.80%	4.794%
28	5.292	1223	1229	1235	rVB3	710	1069	0.08%	0.010%
29	5.324	1235	1239	1241	rBV2	264	218	0.02%	0.002%
30	5.385	1254	1258	1259	rBV2	306	201	0.02%	0.002%
31	5.729	1342	1365	1394	rBV2	493348	1332326	100.00%	12.043%
32	5.867	1406	1408	1415	rVB3	557	419	0.03%	0.004%
33	5.948	1431	1433	1439	rVB2	255	233	0.02%	0.002%
34	5.977	1439	1442	1444	rBV3	251	186	0.01%	0.002%
35	6.047	1461	1464	1470	rVB3	407	435	0.03%	0.004%
36	6.112	1477	1484	1486	rBV3	405	405	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047698.D
 Acq On : 26 Mar 2022 10:55
 Operator : SY/MD
 Sample : VU0326WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK073

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.253	1511	1528	1548	rBV	383817	731974	54.94%	6.616%
38	6.533	1604	1615	1618	rBV5	1669	2382	0.18%	0.022%
39	6.623	1641	1643	1648	rBV2	311	245	0.02%	0.002%
40	6.694	1649	1665	1686	rBV	305844	596909	44.80%	5.396%
41	6.874	1716	1721	1723	rBV2	297	312	0.02%	0.003%
42	7.057	1767	1778	1784	rBV3	618	1006	0.08%	0.009%
43	7.186	1812	1818	1829	rVB5	2072	3875	0.29%	0.035%
44	7.231	1829	1832	1837	rBV3	230	238	0.02%	0.002%
45	7.417	1886	1890	1892	rBV3	249	185	0.01%	0.002%
46	7.568	1924	1937	1960	rVV	171830	303720	22.80%	2.745%
47	7.690	1970	1975	1985	rVB7	1884	3290	0.25%	0.030%
48	7.739	1985	1990	1992	rBV3	349	311	0.02%	0.003%
49	7.800	2000	2009	2024	rVB3	4190	7885	0.59%	0.071%
50	7.899	2024	2040	2056	rBV	619270	1076898	80.83%	9.734%
51	8.182	2116	2128	2153	rBV	122948	213322	16.01%	1.928%
52	8.401	2191	2196	2201	rBV4	779	870	0.07%	0.008%
53	8.562	2240	2246	2248	rBV4	1007	830	0.06%	0.008%
54	8.591	2252	2255	2257	rBV2	324	200	0.02%	0.002%
55	8.639	2257	2270	2308	rBV	511876	947561	71.12%	8.565%
56	8.928	2354	2360	2365	rBV3	569	745	0.06%	0.007%
57	9.018	2385	2388	2395	rVB2	204	246	0.02%	0.002%
58	9.112	2413	2417	2419	rBV2	340	224	0.02%	0.002%
59	9.182	2436	2439	2447	rVB3	309	303	0.02%	0.003%
60	9.420	2499	2513	2547	rBV	576181	969673	72.78%	8.765%
61	9.575	2553	2561	2572	rVB4	2277	3239	0.24%	0.029%
62	9.668	2585	2590	2591	rBV2	260	196	0.01%	0.002%
63	9.693	2591	2598	2607	rBV2	2289	3185	0.24%	0.029%
64	9.784	2622	2626	2628	rBV	316	222	0.02%	0.002%
65	10.028	2698	2702	2706	rVB2	341	297	0.02%	0.003%
66	10.060	2707	2712	2716	rBV3	254	236	0.02%	0.002%
67	10.111	2717	2728	2736	rBV6	2934	5790	0.43%	0.052%
68	10.163	2741	2744	2752	rVB3	185	181	0.01%	0.002%
69	10.292	2780	2784	2789	rVB2	378	423	0.03%	0.004%
70	10.417	2819	2823	2828	rBV2	372	294	0.02%	0.003%
71	10.488	2837	2845	2854	rVV2	2053	2900	0.22%	0.026%
72	10.671	2895	2902	2911	rVB5	1639	2484	0.19%	0.022%
73	10.758	2916	2929	2944	rBV	488164	789658	59.27%	7.138%
74	10.867	2958	2963	2968	rVB2	375	389	0.03%	0.004%
75	10.899	2968	2973	2976	rVV3	581	518	0.04%	0.005%
76	10.922	2976	2980	2984	rVV3	346	365	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047698.D
 Acq On : 26 Mar 2022 10:55
 Operator : SY/MD
 Sample : VU0326WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK073

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.018	3005	3010	3015	rVB2	273	292	0.02%	0.003%
78	11.089	3026	3032	3041	rVB5	1648	2291	0.17%	0.021%
79	11.353	3110	3114	3117	rBV2	297	297	0.02%	0.003%
80	11.472	3140	3151	3168	rVB3	4548	8063	0.61%	0.073%
81	11.578	3180	3184	3191	rVB3	299	326	0.02%	0.003%
82	11.661	3208	3210	3215	rVB2	370	268	0.02%	0.002%
83	11.697	3215	3221	3227	rBV3	943	1253	0.09%	0.011%
84	11.745	3230	3236	3245	rBV2	3708	5420	0.41%	0.049%
85	11.812	3245	3257	3276	rBV	657724	1045551	78.48%	9.451%
86	11.918	3288	3290	3292	rBV3	364	207	0.02%	0.002%
87	12.118	3348	3352	3355	rBV2	298	213	0.02%	0.002%
88	12.195	3360	3376	3399	rBV	663852	1090774	81.87%	9.860%
89	12.427	3445	3448	3451	rBV3	423	275	0.02%	0.002%
90	12.629	3505	3511	3515	rBV2	341	467	0.04%	0.004%
91	13.002	3620	3627	3634	rBV4	1809	2614	0.20%	0.024%
92	13.156	3673	3675	3681	rVB2	246	202	0.02%	0.002%
93	13.221	3686	3695	3707	rVV3	7480	11134	0.84%	0.101%
94	13.844	3879	3889	3900	rBV3	13499	19350	1.45%	0.175%
95	14.089	3955	3965	3981	rBV	41002	66546	4.99%	0.602%
96	14.333	4030	4041	4053	rVB3	15463	24354	1.83%	0.220%
97	14.780	4177	4180	4191	rVB3	556	693	0.05%	0.006%
98	14.835	4192	4197	4202	rBV3	612	742	0.06%	0.007%
99	15.414	4374	4377	4381	rBV3	518	352	0.03%	0.003%
100	15.552	4418	4420	4424	rVB3	747	486	0.04%	0.004%


Sum of corrected areas: 11063023

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047698.D
Acq On : 26 Mar 2022 10:55
Operator : SY/MD
Sample : VU0326WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK073

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

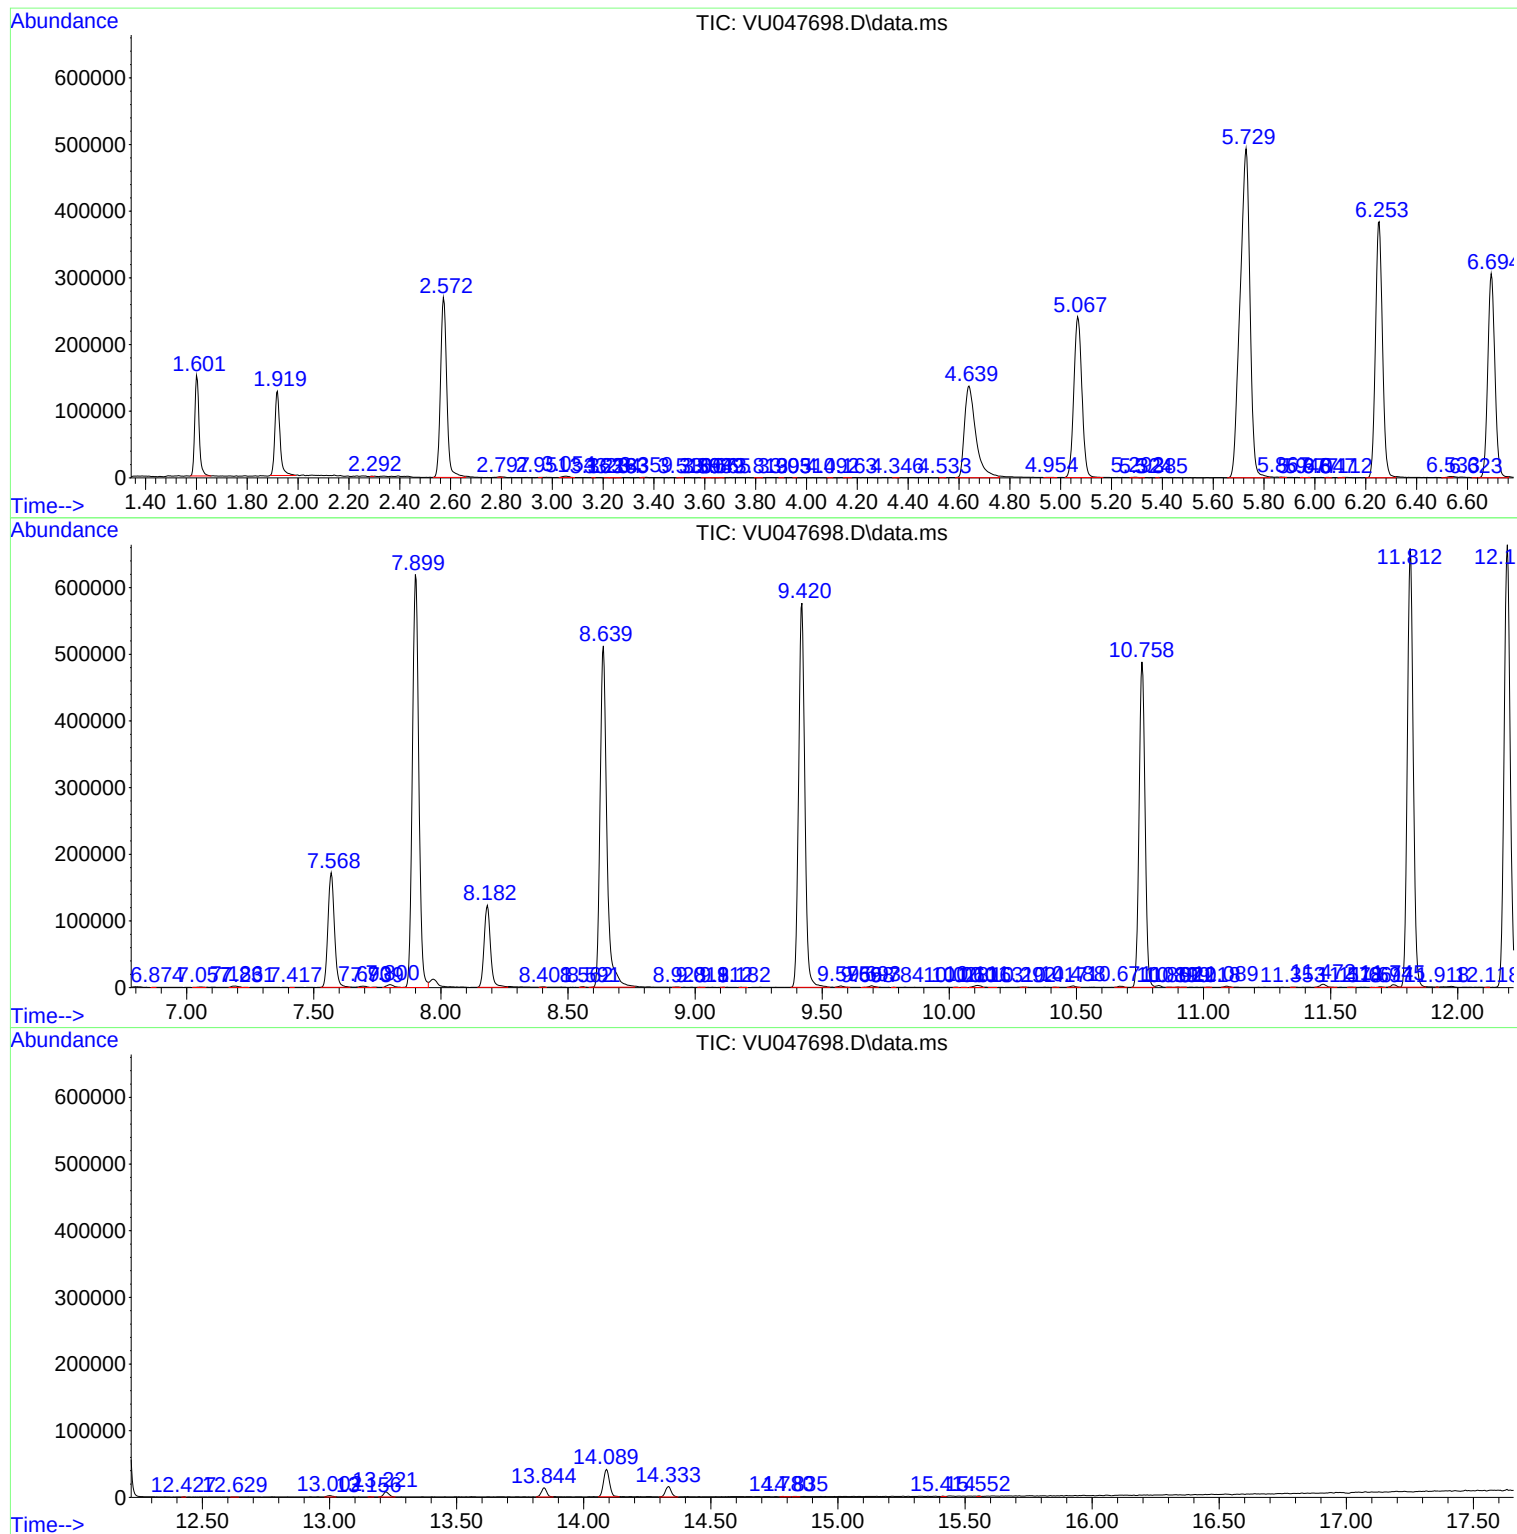

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047698.D
Acq On : 26 Mar 2022 10:55
Operator : SY/MD
Sample : VU0326WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK073

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047698.D
Acq On : 26 Mar 2022 10:55
Operator : SY/MD
Sample : VU0326WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK073

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------