

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047703.D
 Acq On : 26 Mar 2022 13:04
 Operator : SY/MD
 Sample : N2082-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW601

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047703.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	20	rVB2	12867	13660	1.35%	0.138%
2	1.600	73	81	98	rBV	98675	122581	12.12%	1.240%
3	1.919	171	180	198	rBV	80974	115521	11.42%	1.169%
4	2.572	371	383	404	rBV	185602	314196	31.07%	3.179%
5	2.732	431	433	436	rVB2	493	278	0.03%	0.003%
6	2.793	447	452	463	rVB2	1142	2024	0.20%	0.020%
7	3.028	520	525	527	rBV2	328	312	0.03%	0.003%
8	3.044	527	530	531	rBV	362	198	0.02%	0.002%
9	3.125	548	555	559	rVV4	276	360	0.04%	0.004%
10	3.186	570	574	578	rBV3	474	467	0.05%	0.005%
11	3.205	578	580	584	rVB3	623	416	0.04%	0.004%
12	3.231	584	588	591	rBV2	241	157	0.02%	0.002%
13	3.311	610	613	615	rVV	294	190	0.02%	0.002%
14	3.359	617	628	644	rVB3	7965	15916	1.57%	0.161%
15	3.424	644	648	650	rBV	377	263	0.03%	0.003%
16	3.443	650	654	658	rVB2	192	191	0.02%	0.002%
17	3.465	658	661	665	rVB3	330	282	0.03%	0.003%
18	3.485	665	667	672	rVB2	294	193	0.02%	0.002%
19	3.526	672	680	684	rBV3	378	571	0.06%	0.006%
20	3.636	711	714	718	rVB3	324	230	0.02%	0.002%
21	3.803	760	766	771	rBV2	234	270	0.03%	0.003%
22	3.874	771	788	813	rVV2	151301	362873	35.89%	3.672%
23	4.083	847	853	856	rVB3	314	332	0.03%	0.003%
24	4.102	856	859	864	rBV	256	315	0.03%	0.003%
25	4.665	1009	1034	1072	rBV2	132287	498528	49.30%	5.044%
26	4.903	1106	1108	1113	rVB3	417	306	0.03%	0.003%
27	5.012	1138	1142	1143	rBV3	272	196	0.02%	0.002%
28	5.067	1143	1159	1182	rVV	172742	380365	37.62%	3.849%
29	5.247	1213	1215	1217	rBV	335	181	0.02%	0.002%
30	5.321	1220	1238	1258	rBV	318178	717397	70.95%	7.259%
31	5.523	1296	1301	1306	rVB2	464	342	0.03%	0.003%
32	5.552	1306	1310	1312	rBV	198	179	0.02%	0.002%
33	5.729	1343	1365	1399	rBV2	336396	924473	91.43%	9.354%
34	6.047	1461	1464	1467	rVV3	354	194	0.02%	0.002%
35	6.250	1513	1527	1552	rBV	371985	711520	70.37%	7.199%
36	6.546	1609	1619	1630	rBV2	13943	26148	2.59%	0.265%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047703.D
 Acq On : 26 Mar 2022 13:04
 Operator : SY/MD
 Sample : N2082-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW601

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.587	1630	1632	1636	rVB2	549	204	0.02%	0.002%
38	6.694	1650	1665	1684	rBV	216363	421561	41.69%	4.266%
39	6.941	1739	1742	1745	rBV2	209	156	0.02%	0.002%
40	7.018	1762	1766	1769	rBV2	297	272	0.03%	0.003%
41	7.041	1769	1773	1774	rBV	446	370	0.04%	0.004%
42	7.112	1792	1795	1798	rVB2	282	172	0.02%	0.002%
43	7.189	1812	1819	1825	rVV3	771	1120	0.11%	0.011%
44	7.227	1829	1831	1835	rVB	323	178	0.02%	0.002%
45	7.295	1847	1852	1855	rBV	194	172	0.02%	0.002%
46	7.359	1869	1872	1879	rVB2	313	281	0.03%	0.003%
47	7.394	1879	1883	1885	rBV2	245	203	0.02%	0.002%
48	7.568	1924	1937	1957	rBV2	118956	212581	21.02%	2.151%
49	7.793	1997	2007	2009	rBV2	1837	1979	0.20%	0.020%
50	7.899	2026	2040	2055	rBV	417617	727595	71.96%	7.362%
51	8.179	2116	2127	2150	rBV	85797	149554	14.79%	1.513%
52	8.365	2183	2185	2189	rVB2	377	228	0.02%	0.002%
53	8.404	2194	2197	2198	rBV2	287	156	0.02%	0.002%
54	8.475	2204	2219	2229	rBV2	6210	11406	1.13%	0.115%
55	8.555	2233	2244	2257	rBV2	52827	86794	8.58%	0.878%
56	8.639	2257	2270	2303	rBV	341179	657266	65.00%	6.651%
57	8.790	2315	2317	2322	rVB3	776	474	0.05%	0.005%
58	9.009	2380	2385	2388	rBV2	333	317	0.03%	0.003%
59	9.111	2411	2417	2419	rBV3	378	373	0.04%	0.004%
60	9.285	2466	2471	2474	rBV	320	373	0.04%	0.004%
61	9.314	2477	2480	2484	rBV3	211	158	0.02%	0.002%
62	9.417	2499	2512	2539	rBV	561761	941200	93.08%	9.523%
63	9.571	2553	2560	2567	rBV	1809	2302	0.23%	0.023%
64	9.693	2590	2598	2609	rVB3	2916	4445	0.44%	0.045%
65	9.809	2630	2634	2637	rVB2	237	203	0.02%	0.002%
66	9.848	2644	2646	2650	rBV2	180	159	0.02%	0.002%
67	10.111	2718	2728	2738	rBV7	2501	4528	0.45%	0.046%
68	10.266	2773	2776	2779	rVV2	266	196	0.02%	0.002%
69	10.488	2841	2845	2855	rVB3	854	1085	0.11%	0.011%
70	10.635	2887	2891	2895	rBV2	190	182	0.02%	0.002%
71	10.668	2895	2901	2902	rBV	1783	1364	0.13%	0.014%
72	10.758	2916	2929	2946	rBV	359232	583218	57.68%	5.901%
73	10.861	2958	2961	2962	rBV2	514	271	0.03%	0.003%
74	10.896	2962	2972	2984	rVB2	9932	16145	1.60%	0.163%
75	10.973	2993	2996	3001	rVB2	269	257	0.03%	0.003%
76	11.095	3027	3034	3041	rVV3	872	1222	0.12%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047703.D
 Acq On : 26 Mar 2022 13:04
 Operator : SY/MD
 Sample : N2082-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW601

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.208	3065	3069	3072	rBV3	204	179	0.02%	0.002%
78	11.401	3126	3129	3132	rBV3	351	214	0.02%	0.002%
79	11.468	3139	3150	3157	rBV6	2992	4632	0.46%	0.047%
80	11.584	3180	3186	3191	rBV2	334	387	0.04%	0.004%
81	11.655	3206	3208	3213	rVB2	291	184	0.02%	0.002%
82	11.697	3213	3221	3230	rBV4	843	1042	0.10%	0.011%
83	11.748	3230	3237	3245	rVB6	1821	2546	0.25%	0.026%
84	11.812	3245	3257	3281	rBV	631445	1011159	100.00%	10.231%
85	11.947	3292	3299	3301	rBV4	751	849	0.08%	0.009%
86	12.034	3324	3326	3331	rVB3	256	199	0.02%	0.002%
87	12.192	3363	3375	3395	rBV	480653	777435	76.89%	7.866%
88	12.330	3414	3418	3423	rVB3	443	425	0.04%	0.004%
89	12.420	3440	3446	3447	rBV2	354	327	0.03%	0.003%
90	12.594	3497	3500	3502	rBV2	257	186	0.02%	0.002%
91	12.668	3519	3523	3525	rBV3	260	190	0.02%	0.002%
92	12.706	3533	3535	3538	rBV	327	197	0.02%	0.002%
93	12.774	3547	3556	3565	rVB4	1996	3377	0.33%	0.034%
94	12.832	3572	3574	3578	rVB2	294	165	0.02%	0.002%
95	13.224	3688	3696	3707	rVB5	3192	4580	0.45%	0.046%
96	13.272	3708	3711	3715	rBV2	260	243	0.02%	0.002%
97	13.417	3753	3756	3759	rBV2	195	180	0.02%	0.002%
98	13.844	3881	3889	3900	rVB5	4631	6841	0.68%	0.069%
99	14.092	3957	3966	3978	rBV2	11452	18248	1.80%	0.185%
100	14.330	4033	4040	4051	rVB3	4864	6808	0.67%	0.069%




Sum of corrected areas: 9882938

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047703.D
Acq On : 26 Mar 2022 13:04
Operator : SY/MD
Sample : N2082-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW601

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

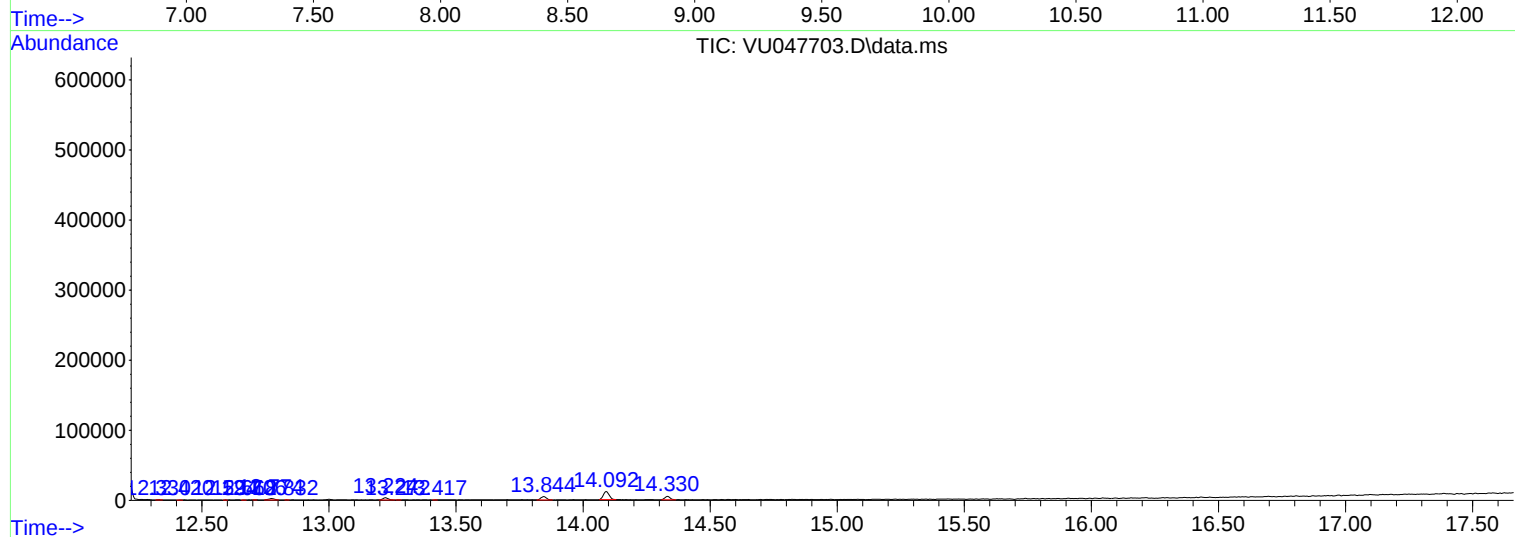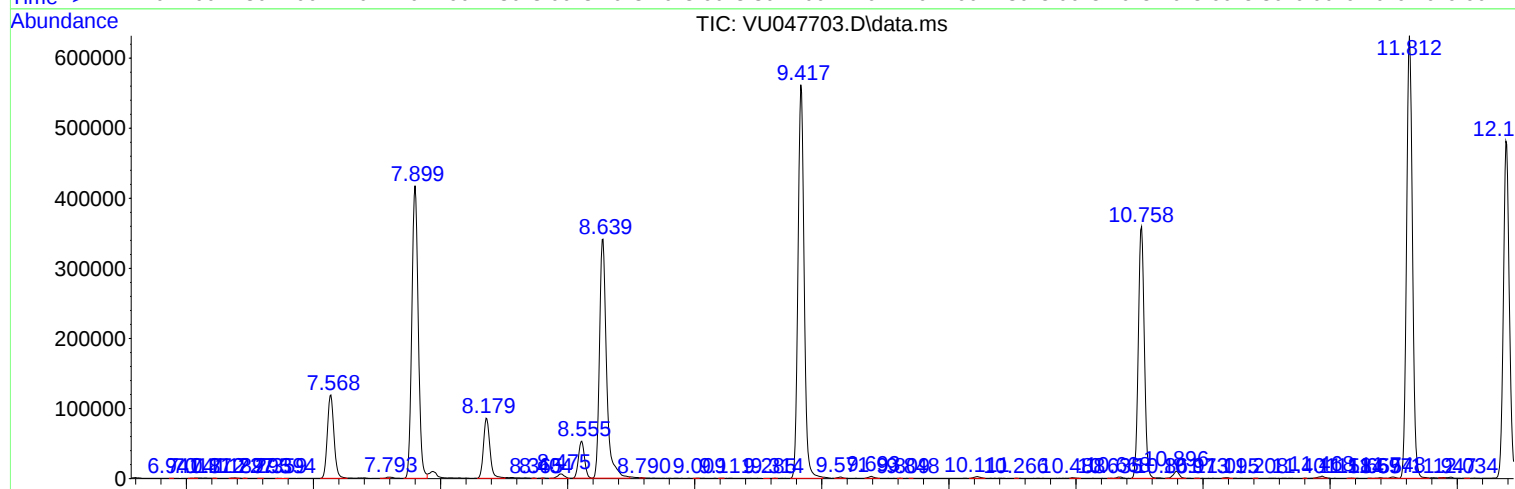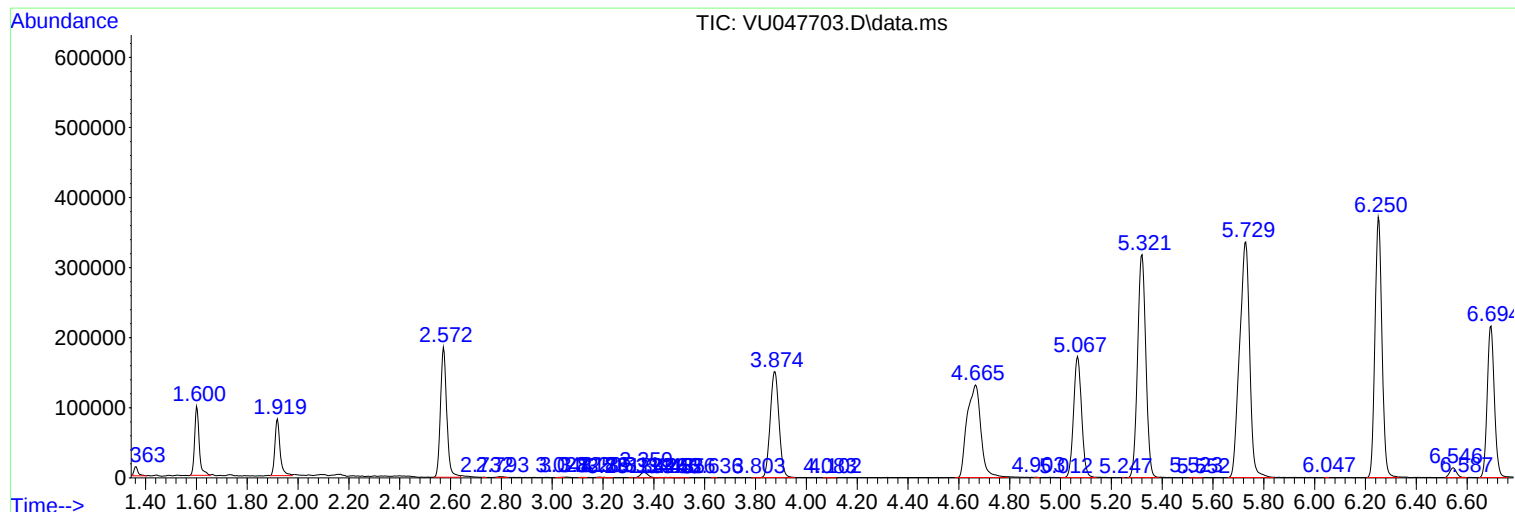

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047703.D
Acq On : 26 Mar 2022 13:04
Operator : SY/MD
Sample : N2082-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW601

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047703.D
Acq On : 26 Mar 2022 13:04
Operator : SY/MD
Sample : N2082-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW601

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------