

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047706.D
 Acq On : 26 Mar 2022 14:11
 Operator : SY/MD
 Sample : N2081-02DL 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047706.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	99	rBV	95528	117147	11.50%	1.319%
2	1.916	171	179	200	rBV2	92892	170805	16.77%	1.923%
3	2.572	370	383	416	rVV	180397	310059	30.44%	3.490%
4	2.687	416	419	422	rVB2	353	243	0.02%	0.003%
5	2.771	442	445	446	rBV2	436	268	0.03%	0.003%
6	2.790	446	451	458	rBV2	587	848	0.08%	0.010%
7	2.964	502	505	508	rBV	423	290	0.03%	0.003%
8	3.054	525	533	542	rVV2	1134	2026	0.20%	0.023%
9	3.138	553	559	561	rBV3	280	267	0.03%	0.003%
10	3.363	623	629	638	rVB2	875	1158	0.11%	0.013%
11	3.459	656	659	662	rVB	325	194	0.02%	0.002%
12	3.591	695	700	704	rVB2	327	296	0.03%	0.003%
13	3.620	704	709	712	rBV2	225	268	0.03%	0.003%
14	3.874	773	788	805	rBV	26370	61546	6.04%	0.693%
15	3.996	820	826	827	rBV2	293	260	0.03%	0.003%
16	4.047	836	842	844	rBV2	160	192	0.02%	0.002%
17	4.067	845	848	853	rVV3	295	268	0.03%	0.003%
18	4.121	862	865	868	rVV2	233	193	0.02%	0.002%
19	4.176	878	882	886	rBV3	261	200	0.02%	0.002%
20	4.237	897	901	905	rBV3	285	253	0.02%	0.003%
21	4.337	929	932	936	rVB	334	293	0.03%	0.003%
22	4.494	978	981	984	rBV	230	206	0.02%	0.002%
23	4.572	1000	1005	1008	rBV2	397	328	0.03%	0.004%
24	4.636	1011	1025	1058	rBV2	109123	398058	39.08%	4.481%
25	5.067	1142	1159	1177	rBV	171109	378094	37.12%	4.256%
26	5.247	1212	1215	1221	rVV3	258	199	0.02%	0.002%
27	5.318	1221	1237	1259	rVB	87336	199565	19.59%	2.246%
28	5.726	1341	1364	1395	rBV2	332389	912140	89.56%	10.267%
29	5.957	1432	1436	1439	rVV4	403	310	0.03%	0.003%
30	5.983	1439	1444	1448	rVV3	655	681	0.07%	0.008%
31	6.131	1488	1490	1495	rVB2	395	252	0.02%	0.003%
32	6.250	1511	1527	1549	rBV	385180	720630	70.75%	8.112%
33	6.543	1607	1618	1626	rVV5	2726	4807	0.47%	0.054%
34	6.690	1650	1664	1687	rBV	217789	423873	41.62%	4.771%
35	6.809	1698	1701	1708	rVB4	549	496	0.05%	0.006%
36	6.887	1723	1725	1731	rBV2	221	251	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047706.D
 Acq On : 26 Mar 2022 14:11
 Operator : SY/MD
 Sample : N2081-02DL 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.009	1759	1763	1770	rVV3	319	327	0.03%	0.004%
38	7.041	1770	1773	1774	rBV3	344	202	0.02%	0.002%
39	7.137	1798	1803	1808	rBV3	214	205	0.02%	0.002%
40	7.186	1814	1818	1819	rBV3	727	425	0.04%	0.005%
41	7.276	1843	1846	1851	rVB2	254	245	0.02%	0.003%
42	7.565	1918	1936	1960	rBV	119014	212588	20.87%	2.393%
43	7.803	2002	2010	2013	rBV5	424	576	0.06%	0.006%
44	7.899	2026	2040	2055	rBV	413871	719615	70.65%	8.100%
45	8.099	2100	2102	2105	rVB2	421	242	0.02%	0.003%
46	8.124	2105	2110	2114	rVB3	311	241	0.02%	0.003%
47	8.179	2114	2127	2145	rBV	85188	147654	14.50%	1.662%
48	8.346	2177	2179	2185	rVB2	560	481	0.05%	0.005%
49	8.475	2209	2219	2224	rBV3	1672	2167	0.21%	0.024%
50	8.552	2235	2243	2254	rVB6	4367	6626	0.65%	0.075%
51	8.639	2257	2270	2303	rBV	358960	677607	66.53%	7.627%
52	9.018	2382	2388	2392	rVB2	331	383	0.04%	0.004%
53	9.089	2404	2410	2412	rBV2	220	201	0.02%	0.002%
54	9.211	2444	2448	2450	rBV	264	202	0.02%	0.002%
55	9.330	2481	2485	2488	rBV2	362	327	0.03%	0.004%
56	9.417	2498	2512	2548	rBV	565986	952743	93.54%	10.724%
57	9.571	2553	2560	2571	rVB2	2268	3149	0.31%	0.035%
58	9.690	2589	2597	2611	rBV3	4495	6910	0.68%	0.078%
59	9.829	2634	2640	2644	rBV3	325	435	0.04%	0.005%
60	9.861	2647	2650	2655	rVV2	255	274	0.03%	0.003%
61	10.105	2716	2726	2734	rVV3	2838	4281	0.42%	0.048%
62	10.282	2776	2781	2787	rBV2	239	280	0.03%	0.003%
63	10.324	2788	2794	2797	rVB2	347	339	0.03%	0.004%
64	10.491	2835	2846	2851	rVV3	782	1150	0.11%	0.013%
65	10.581	2869	2874	2880	rBV3	228	276	0.03%	0.003%
66	10.636	2886	2891	2893	rBV2	326	229	0.02%	0.003%
67	10.674	2895	2903	2909	rVB3	1982	2371	0.23%	0.027%
68	10.758	2914	2929	2947	rBV	375415	602200	59.13%	6.778%
69	10.893	2962	2971	2972	rBV4	1883	1767	0.17%	0.020%
70	10.999	2994	3004	3011	rBV4	1649	2746	0.27%	0.031%
71	11.089	3025	3032	3039	rBV2	1277	1870	0.18%	0.021%
72	11.140	3045	3048	3055	rVB	355	257	0.03%	0.003%
73	11.295	3088	3096	3106	rVB3	1285	2047	0.20%	0.023%
74	11.468	3139	3150	3162	rVB4	6771	10991	1.08%	0.124%
75	11.681	3212	3216	3218	rBV3	296	223	0.02%	0.003%
76	11.742	3231	3235	3237	rBV3	571	395	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047706.D
 Acq On : 26 Mar 2022 14:11
 Operator : SY/MD
 Sample : N2081-02DL 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.812	3243	3257	3275	rBV	644415	1018511	100.00%	11.465%
78	11.925	3289	3292	3294	rBV4	579	338	0.03%	0.004%
79	11.941	3295	3297	3300	rVB2	851	413	0.04%	0.005%
80	11.970	3303	3306	3313	rVB3	1426	1520	0.15%	0.017%
81	12.002	3313	3316	3320	rVB2	368	225	0.02%	0.003%
82	12.031	3322	3325	3329	rVB2	294	201	0.02%	0.002%
83	12.086	3338	3342	3343	rBV3	647	399	0.04%	0.004%
84	12.192	3361	3375	3397	rBV	479845	777772	76.36%	8.755%
85	12.372	3429	3431	3436	rVB3	339	289	0.03%	0.003%
86	12.398	3436	3439	3441	rBV	414	259	0.03%	0.003%
87	12.478	3458	3464	3468	rBV3	389	560	0.05%	0.006%
88	12.642	3510	3515	3518	rBV2	526	595	0.06%	0.007%
89	12.777	3549	3557	3561	rBV4	848	1384	0.14%	0.016%
90	13.034	3633	3637	3642	rBV3	471	356	0.03%	0.004%
91	13.160	3672	3676	3680	rBV3	421	460	0.05%	0.005%
92	13.295	3715	3718	3727	rVB2	477	419	0.04%	0.005%
93	13.455	3766	3768	3777	rVB4	501	601	0.06%	0.007%
94	13.848	3885	3890	3901	rVB3	1566	2003	0.20%	0.023%
95	13.893	3901	3904	3907	rBV	237	201	0.02%	0.002%
96	13.992	3932	3935	3939	rBV3	272	275	0.03%	0.003%
97	14.092	3960	3966	3973	rBV3	2313	2692	0.26%	0.030%
98	14.333	4035	4041	4048	rBV2	1285	1659	0.16%	0.019%
99	14.799	4184	4186	4190	rBV2	407	324	0.03%	0.004%
100	14.967	4234	4238	4241	rVB3	405	343	0.03%	0.004%




Sum of corrected areas: 8884010

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047706.D
Acq On : 26 Mar 2022 14:11
Operator : SY/MD
Sample : N2081-02DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

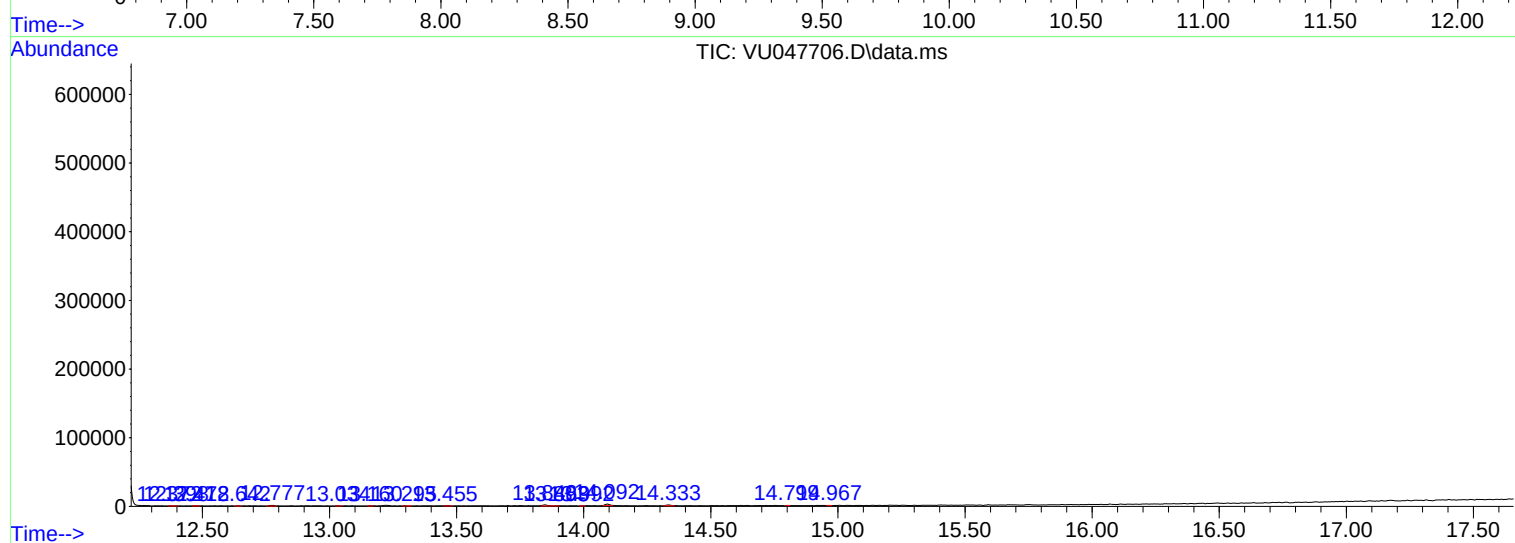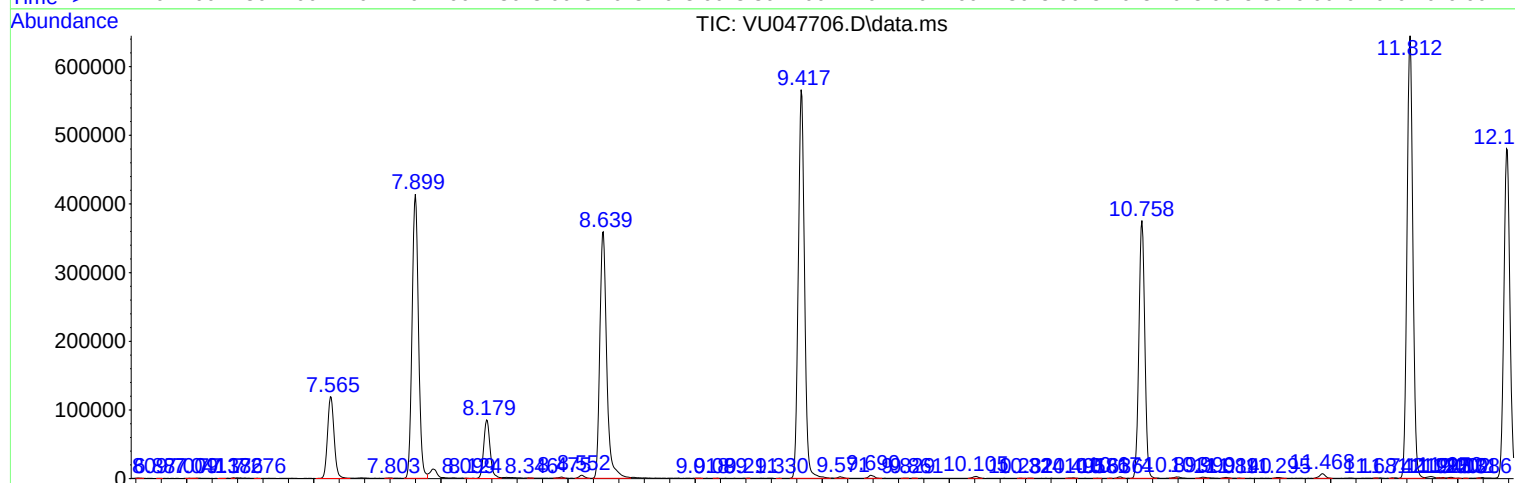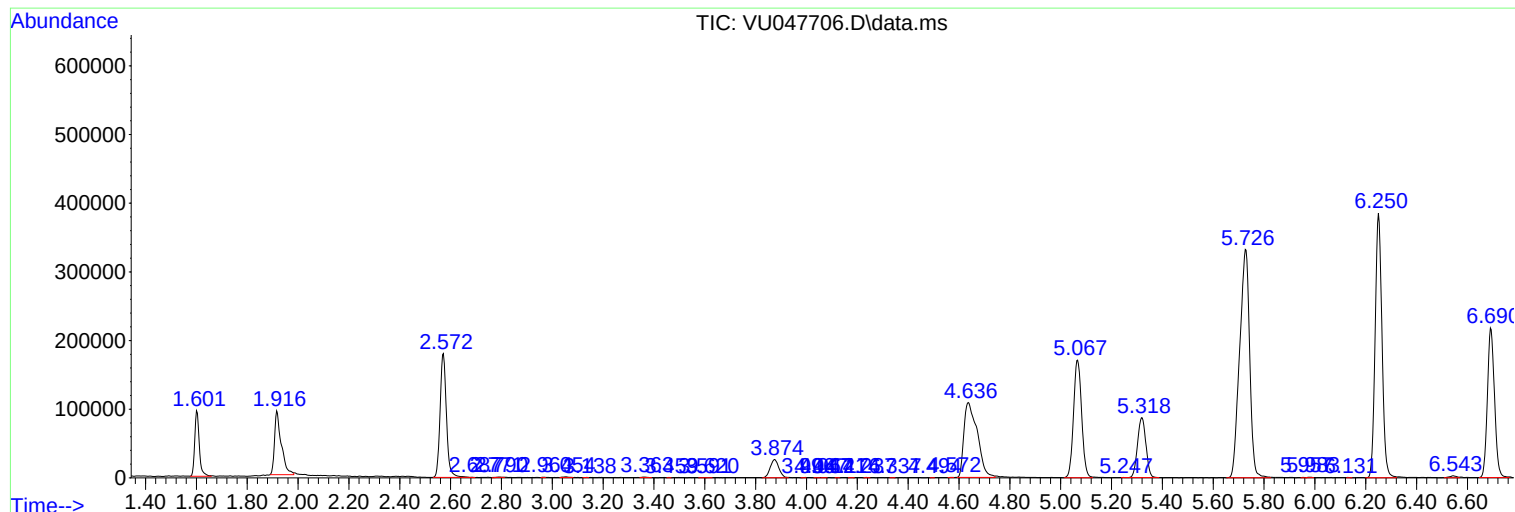

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047706.D
Acq On : 26 Mar 2022 14:11
Operator : SY/MD
Sample : N2081-02DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047706.D
Acq On : 26 Mar 2022 14:11
Operator : SY/MD
Sample : N2081-02DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------