

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047708.D
 Acq On : 26 Mar 2022 14:57
 Operator : SY/MD
 Sample : N2081-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047708.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	71	81	101	rVB	100077	132521	6.16%	1.122%
2	1.919	171	180	209	rVB2	82294	178247	8.29%	1.509%
3	2.572	371	383	400	rBV2	182642	322680	15.01%	2.731%
4	2.928	484	494	496	rBV3	2780	4097	0.19%	0.035%
5	3.047	525	531	535	rBV5	515	640	0.03%	0.005%
6	3.250	589	594	597	rBV4	433	503	0.02%	0.004%
7	3.279	600	603	609	rVB3	505	554	0.03%	0.005%
8	3.318	610	615	616	rBV2	673	513	0.02%	0.004%
9	3.363	621	629	646	rVB6	5778	13018	0.61%	0.110%
10	3.440	648	653	656	rVB2	295	261	0.01%	0.002%
11	3.485	664	667	671	rVB2	387	356	0.02%	0.003%
12	3.581	693	697	701	rBV2	267	287	0.01%	0.002%
13	3.874	771	788	806	rBV	169672	402947	18.74%	3.411%
14	4.131	864	868	872	rBV	409	370	0.02%	0.003%
15	4.282	912	915	920	rVB	327	308	0.01%	0.003%
16	4.578	999	1007	1011	rBV3	1419	2152	0.10%	0.018%
17	4.668	1011	1035	1076	rVV2	259018	818508	38.08%	6.928%
18	4.835	1085	1087	1091	rVB2	661	350	0.02%	0.003%
19	5.063	1142	1158	1203	rBV2	279074	658597	30.64%	5.575%
20	5.247	1213	1215	1219	rVB2	465	297	0.01%	0.003%
21	5.321	1219	1238	1258	rBV	959868	2149704	100.00%	18.196%
22	5.726	1342	1364	1399	rBV2	321827	882429	41.05%	7.469%
23	5.903	1417	1419	1424	rVB2	411	284	0.01%	0.002%
24	5.967	1436	1439	1441	rBV2	490	317	0.01%	0.003%
25	5.989	1444	1446	1452	rVB2	467	337	0.02%	0.003%
26	6.038	1458	1461	1464	rBV2	383	253	0.01%	0.002%
27	6.250	1512	1527	1551	rBV	367174	693966	32.28%	5.874%
28	6.469	1592	1595	1602	rVB2	307	339	0.02%	0.003%
29	6.542	1608	1618	1634	rVB3	16883	32958	1.53%	0.279%
30	6.694	1650	1665	1680	rBV	207830	404577	18.82%	3.425%
31	6.809	1699	1701	1707	rVB4	809	764	0.04%	0.006%
32	7.005	1759	1762	1767	rVB3	292	250	0.01%	0.002%
33	7.044	1768	1774	1776	rBV2	432	392	0.02%	0.003%
34	7.086	1782	1787	1791	rBV3	357	457	0.02%	0.004%
35	7.147	1801	1806	1809	rBV2	344	413	0.02%	0.003%
36	7.189	1812	1819	1823	rBV4	880	1152	0.05%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047708.D
 Acq On : 26 Mar 2022 14:57
 Operator : SY/MD
 Sample : N2081-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.256	1837	1840	1848	rVB2	383	409	0.02%	0.003%
38	7.295	1848	1852	1857	rBV2	302	268	0.01%	0.002%
39	7.443	1892	1898	1901	rBV2	344	386	0.02%	0.003%
40	7.497	1913	1915	1920	rBV3	494	491	0.02%	0.004%
41	7.568	1925	1937	1953	rBV	116417	205878	9.58%	1.743%
42	7.758	1991	1996	1998	rBV2	317	296	0.01%	0.003%
43	7.796	2004	2008	2010	rBV3	725	569	0.03%	0.005%
44	7.899	2026	2040	2055	rBV	400145	693171	32.24%	5.867%
45	8.031	2078	2081	2092	rVB6	1239	1685	0.08%	0.014%
46	8.092	2097	2100	2106	rVB4	747	791	0.04%	0.007%
47	8.179	2116	2127	2144	rBV	80403	140271	6.53%	1.187%
48	8.430	2201	2205	2207	rBV3	322	294	0.01%	0.002%
49	8.475	2211	2219	2232	rVB2	3028	5213	0.24%	0.044%
50	8.555	2232	2244	2257	rBV	100747	170274	7.92%	1.441%
51	8.636	2257	2269	2301	rBV	339093	631158	29.36%	5.342%
52	8.809	2321	2323	2325	rVB2	668	299	0.01%	0.003%
53	8.867	2333	2341	2349	rBV5	1578	2480	0.12%	0.021%
54	8.922	2353	2358	2359	rBV4	654	477	0.02%	0.004%
55	9.263	2459	2464	2466	rBV	251	256	0.01%	0.002%
56	9.317	2478	2481	2488	rBV2	250	353	0.02%	0.003%
57	9.417	2498	2512	2539	rBV	532714	906283	42.16%	7.671%
58	9.571	2556	2560	2563	rBV2	856	646	0.03%	0.005%
59	9.687	2588	2596	2597	rBV3	1470	1197	0.06%	0.010%
60	9.777	2619	2624	2628	rBV2	535	534	0.02%	0.005%
61	9.883	2652	2657	2662	rVV2	529	628	0.03%	0.005%
62	9.902	2662	2663	2669	rVB3	482	285	0.01%	0.002%
63	10.015	2693	2698	2700	rBV2	456	330	0.02%	0.003%
64	10.063	2711	2713	2720	rVB3	390	287	0.01%	0.002%
65	10.099	2721	2724	2727	rVV3	547	523	0.02%	0.004%
66	10.269	2771	2777	2788	rVB6	2833	3990	0.19%	0.034%
67	10.362	2803	2806	2808	rBV	510	272	0.01%	0.002%
68	10.420	2820	2824	2829	rVB2	473	486	0.02%	0.004%
69	10.484	2841	2844	2850	rVB2	697	650	0.03%	0.006%
70	10.591	2873	2877	2879	rBV	384	314	0.01%	0.003%
71	10.671	2898	2902	2905	rBV3	1306	1117	0.05%	0.009%
72	10.758	2916	2929	2946	rBV	344213	558573	25.98%	4.728%
73	10.819	2946	2948	2955	rVB4	949	601	0.03%	0.005%
74	10.896	2958	2972	2987	rVB2	5830	10620	0.49%	0.090%
75	11.086	3025	3031	3038	rBV5	1627	2527	0.12%	0.021%
76	11.298	3086	3097	3108	rBV7	2258	4213	0.20%	0.036%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047708.D
 Acq On : 26 Mar 2022 14:57
 Operator : SY/MD
 Sample : N2081-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.468	3138	3150	3160	rVB5	6210	9934	0.46%	0.084%
78	11.594	3181	3189	3198	rVB7	1349	2212	0.10%	0.019%
79	11.645	3199	3205	3209	rBV3	292	341	0.02%	0.003%
80	11.697	3214	3221	3228	rVB4	1322	1865	0.09%	0.016%
81	11.738	3228	3234	3235	rBV3	822	623	0.03%	0.005%
82	11.812	3244	3257	3275	rBV	615183	965293	44.90%	8.171%
83	11.896	3276	3283	3291	rVB	4274	6158	0.29%	0.052%
84	11.935	3291	3295	3296	rBV2	870	586	0.03%	0.005%
85	12.060	3327	3334	3335	rBV3	773	766	0.04%	0.006%
86	12.095	3339	3345	3347	rBV4	1617	1667	0.08%	0.014%
87	12.192	3360	3375	3394	rBV	461467	753380	35.05%	6.377%
88	12.262	3394	3397	3400	rVV3	547	412	0.02%	0.003%
89	12.320	3412	3415	3417	rVV2	468	321	0.01%	0.003%
90	12.439	3446	3452	3454	rBV2	366	394	0.02%	0.003%
91	12.484	3462	3466	3469	rBV3	463	362	0.02%	0.003%
92	12.642	3512	3515	3522	rVB2	628	528	0.02%	0.004%
93	12.697	3522	3532	3539	rBV7	1787	2971	0.14%	0.025%
94	12.771	3551	3555	3564	rVB3	1126	1465	0.07%	0.012%
95	12.867	3578	3585	3592	rBV3	1781	2062	0.10%	0.017%
96	13.111	3654	3661	3664	rBV4	437	546	0.03%	0.005%
97	13.452	3764	3767	3777	rVB5	1156	1529	0.07%	0.013%
98	13.793	3868	3873	3878	rVB2	963	1024	0.05%	0.009%
99	13.944	3917	3920	3924	rBV2	527	429	0.02%	0.004%
100	14.092	3960	3966	3975	rVB2	3500	4422	0.21%	0.037%




Sum of corrected areas: 11814183

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047708.D
Acq On : 26 Mar 2022 14:57
Operator : SY/MD
Sample : N2081-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

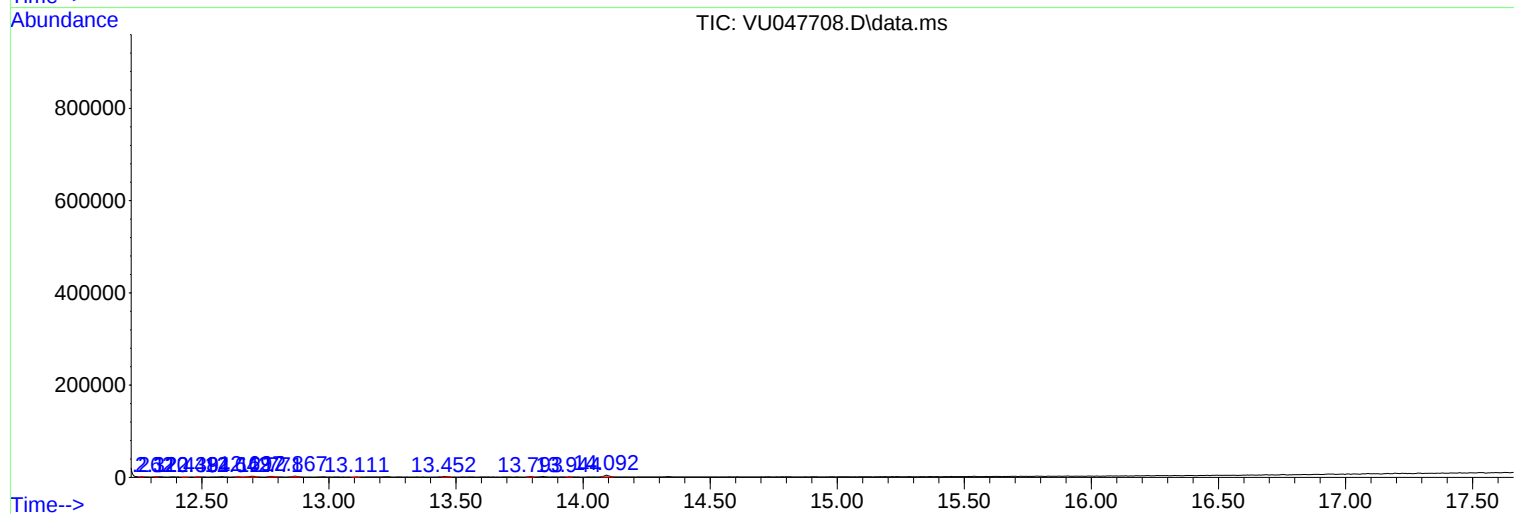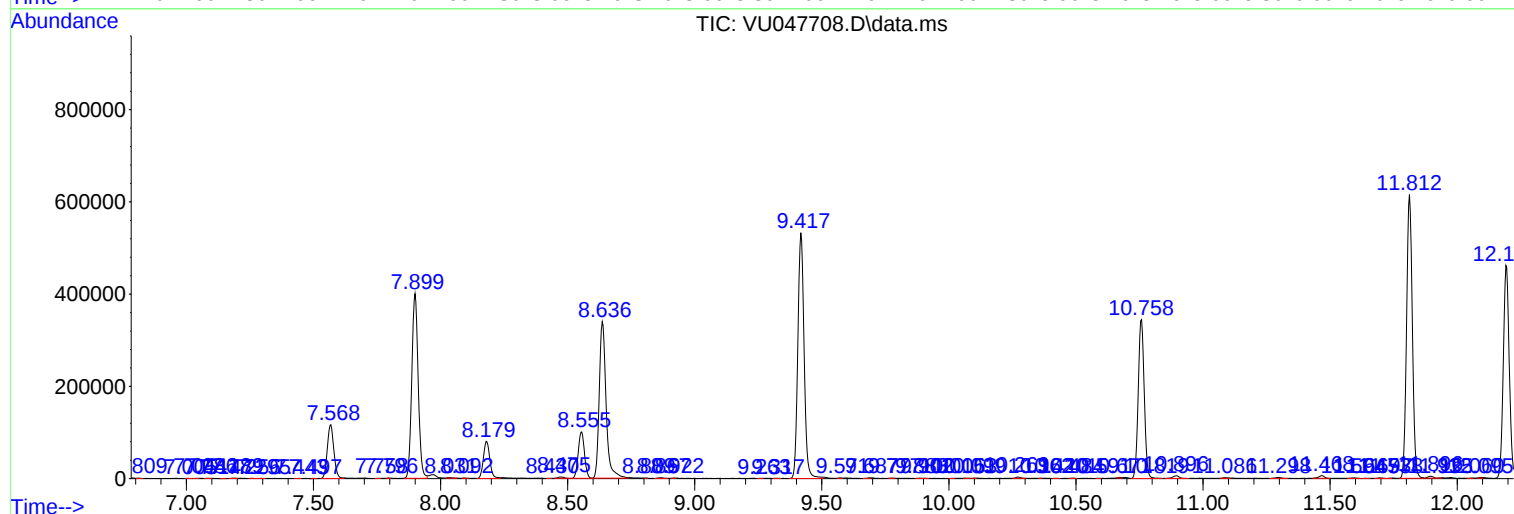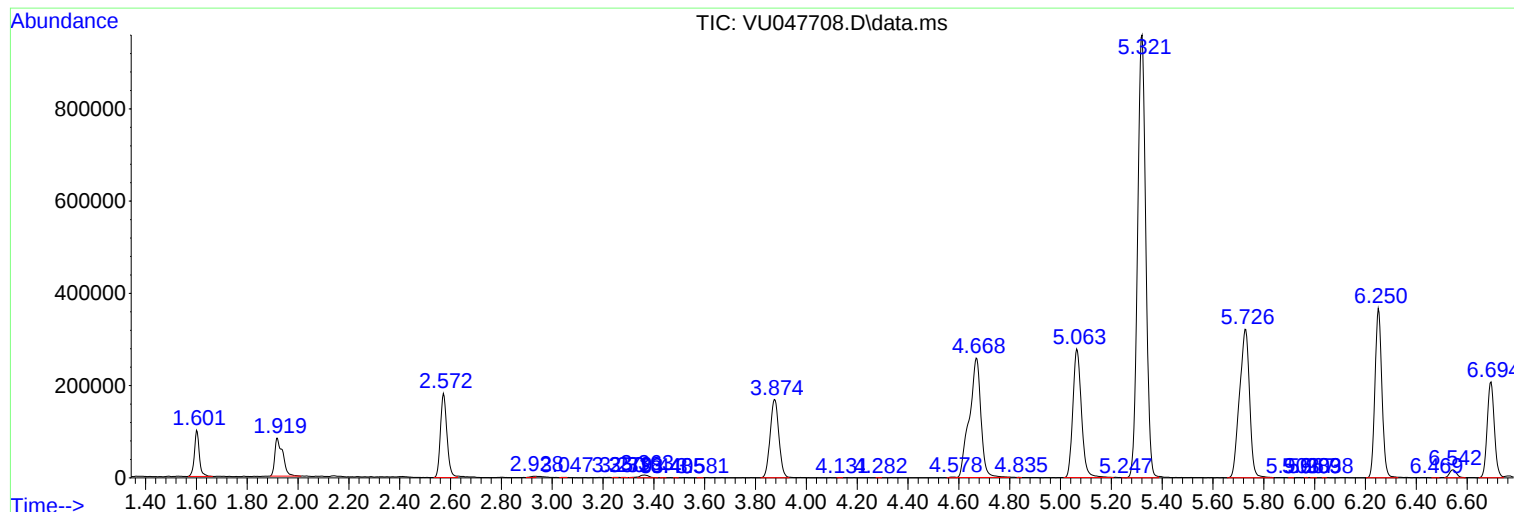

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047708.D
Acq On : 26 Mar 2022 14:57
Operator : SY/MD
Sample : N2081-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047708.D
Acq On : 26 Mar 2022 14:57
Operator : SY/MD
Sample : N2081-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc