

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047709.D
 Acq On : 26 Mar 2022 15:19
 Operator : SY/MD
 Sample : N2081-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047709.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	101	rVB	93276	109600	10.77%	1.141%
2	1.915	171	179	201	rVB	84960	117822	11.57%	1.227%
3	2.362	316	318	321	rBV4	558	280	0.03%	0.003%
4	2.571	370	383	400	rBV2	187784	336199	33.02%	3.501%
5	2.957	500	503	507	rVV3	423	347	0.03%	0.004%
6	2.996	512	515	519	rBV2	332	215	0.02%	0.002%
7	3.038	524	528	530	rBV3	283	203	0.02%	0.002%
8	3.054	530	533	536	rBV2	409	271	0.03%	0.003%
9	3.128	553	556	561	rVB2	401	406	0.04%	0.004%
10	3.160	561	566	569	rBV	490	485	0.05%	0.005%
11	3.186	569	574	582	rVB5	615	1046	0.10%	0.011%
12	3.314	607	614	616	rBV2	252	298	0.03%	0.003%
13	3.362	621	629	640	rVB7	3178	6066	0.60%	0.063%
14	3.610	704	706	709	rVB2	288	200	0.02%	0.002%
15	3.787	756	761	764	rBV	349	266	0.03%	0.003%
16	3.874	772	788	816	rVB	76277	181092	17.79%	1.886%
17	4.121	862	865	868	rVV	276	215	0.02%	0.002%
18	4.179	881	883	890	rVB2	227	219	0.02%	0.002%
19	4.330	926	930	935	rVV	188	213	0.02%	0.002%
20	4.394	946	950	957	rVV2	332	304	0.03%	0.003%
21	4.632	1010	1024	1059	rBV	105661	331981	32.61%	3.457%
22	5.066	1142	1159	1183	rBV	173105	382065	37.53%	3.979%
23	5.320	1219	1238	1257	rBV	453280	1018058	100.00%	10.602%
24	5.513	1296	1298	1301	rBV	352	246	0.02%	0.003%
25	5.529	1301	1303	1308	rVV2	373	289	0.03%	0.003%
26	5.729	1343	1365	1390	rBV2	327191	892876	87.70%	9.299%
27	5.848	1400	1402	1407	rVB2	563	395	0.04%	0.004%
28	5.874	1407	1410	1415	rBV2	300	318	0.03%	0.003%
29	5.983	1440	1444	1448	rVB2	322	220	0.02%	0.002%
30	6.105	1480	1482	1491	rVB2	305	317	0.03%	0.003%
31	6.250	1513	1527	1556	rBV	368895	704888	69.24%	7.341%
32	6.546	1605	1619	1632	rVV3	17727	33231	3.26%	0.346%
33	6.690	1650	1664	1692	rBV	210390	412732	40.54%	4.298%
34	6.809	1695	1701	1704	rVV2	744	812	0.08%	0.008%
35	6.838	1707	1710	1713	rVV	265	222	0.02%	0.002%
36	7.057	1776	1778	1781	rVB	350	207	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047709.D
 Acq On : 26 Mar 2022 15:19
 Operator : SY/MD
 Sample : N2081-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.108	1791	1794	1800	rVB3	366	360	0.04%	0.004%
38	7.137	1800	1803	1807	rBV2	287	252	0.02%	0.003%
39	7.189	1809	1819	1821	rBV4	978	1178	0.12%	0.012%
40	7.568	1923	1937	1957	rBV	114695	206504	20.28%	2.151%
41	7.639	1957	1959	1963	rVB	844	446	0.04%	0.005%
42	7.668	1963	1968	1970	rBV3	574	455	0.04%	0.005%
43	7.687	1971	1974	1980	rVB5	619	656	0.06%	0.007%
44	7.796	2004	2008	2011	rBV3	583	477	0.05%	0.005%
45	7.899	2026	2040	2057	rBV	404230	708094	69.55%	7.374%
46	8.050	2084	2087	2091	rVB3	433	324	0.03%	0.003%
47	8.179	2115	2127	2142	rBV	81601	141739	13.92%	1.476%
48	8.401	2191	2196	2199	rBV3	1162	1085	0.11%	0.011%
49	8.449	2206	2211	2212	rBV	729	417	0.04%	0.004%
50	8.471	2212	2218	2233	rVB2	3549	6112	0.60%	0.064%
51	8.555	2233	2244	2257	rVB	48285	80684	7.93%	0.840%
52	8.635	2257	2269	2296	rBV	348156	642231	63.08%	6.688%
53	8.764	2306	2309	2316	rVB5	970	1050	0.10%	0.011%
54	8.838	2330	2332	2337	rBV3	278	252	0.02%	0.003%
55	8.870	2338	2342	2344	rBV3	395	269	0.03%	0.003%
56	9.012	2380	2386	2389	rBV3	298	262	0.03%	0.003%
57	9.089	2405	2410	2414	rBV2	254	286	0.03%	0.003%
58	9.314	2473	2480	2484	rBV2	290	394	0.04%	0.004%
59	9.417	2499	2512	2551	rBV	551124	935375	91.88%	9.741%
60	9.565	2554	2558	2560	rBV3	402	328	0.03%	0.003%
61	9.690	2591	2597	2598	rBV2	816	657	0.06%	0.007%
62	9.754	2613	2617	2620	rVB	419	299	0.03%	0.003%
63	9.983	2684	2688	2693	rVB2	356	332	0.03%	0.003%
64	10.015	2693	2698	2701	rBV	232	236	0.02%	0.002%
65	10.102	2720	2725	2727	rBV3	308	305	0.03%	0.003%
66	10.179	2745	2749	2753	rVB2	294	246	0.02%	0.003%
67	10.291	2781	2784	2786	rBV2	323	206	0.02%	0.002%
68	10.385	2810	2813	2818	rVB	258	221	0.02%	0.002%
69	10.452	2830	2834	2836	rBV	381	342	0.03%	0.004%
70	10.465	2836	2838	2841	rVV2	388	284	0.03%	0.003%
71	10.484	2841	2844	2848	rVV	400	344	0.03%	0.004%
72	10.510	2848	2852	2857	rVB2	235	264	0.03%	0.003%
73	10.671	2897	2902	2910	rVB4	1429	1508	0.15%	0.016%
74	10.758	2916	2929	2946	rBV	352390	567388	55.73%	5.909%
75	10.822	2947	2949	2953	rVB2	491	331	0.03%	0.003%
76	10.893	2962	2971	2983	rBV2	6591	10962	1.08%	0.114%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047709.D
 Acq On : 26 Mar 2022 15:19
 Operator : SY/MD
 Sample : N2081-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.008	3005	3007	3011	rVB2	410	227	0.02%	0.002%
78	11.095	3030	3034	3038	rBV	294	298	0.03%	0.003%
79	11.156	3050	3053	3058	rVB2	357	258	0.03%	0.003%
80	11.291	3091	3095	3098	rBV2	290	264	0.03%	0.003%
81	11.385	3121	3124	3129	rVB	295	275	0.03%	0.003%
82	11.413	3129	3133	3136	rBV2	269	293	0.03%	0.003%
83	11.468	3141	3150	3160	rBV4	1823	3034	0.30%	0.032%
84	11.700	3217	3222	3226	rVB3	604	563	0.06%	0.006%
85	11.812	3244	3257	3278	rBV	621387	980799	96.34%	10.214%
86	11.918	3287	3290	3293	rBV2	377	264	0.03%	0.003%
87	11.976	3303	3308	3314	rVB3	1273	1583	0.16%	0.016%
88	12.195	3361	3376	3391	rBV	462410	760077	74.66%	7.916%
89	12.336	3415	3420	3423	rVB2	588	485	0.05%	0.005%
90	12.368	3427	3430	3440	rVB3	307	343	0.03%	0.004%
91	12.500	3468	3471	3476	rBV3	522	493	0.05%	0.005%
92	12.536	3476	3482	3485	rVV3	326	366	0.04%	0.004%
93	12.561	3486	3490	3494	rVB2	213	206	0.02%	0.002%
94	12.622	3506	3509	3515	rBV2	230	236	0.02%	0.002%
95	12.777	3549	3557	3565	rVB3	1341	2327	0.23%	0.024%
96	12.909	3593	3598	3600	rBV2	425	332	0.03%	0.003%
97	13.224	3693	3696	3704	rVB3	573	579	0.06%	0.006%
98	13.844	3885	3889	3890	rBV2	529	370	0.04%	0.004%
99	14.333	4036	4041	4042	rBV2	589	499	0.05%	0.005%
100	15.343	4352	4355	4358	rBV3	558	391	0.04%	0.004%




Sum of corrected areas: 9602321

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047709.D
Acq On : 26 Mar 2022 15:19
Operator : SY/MD
Sample : N2081-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

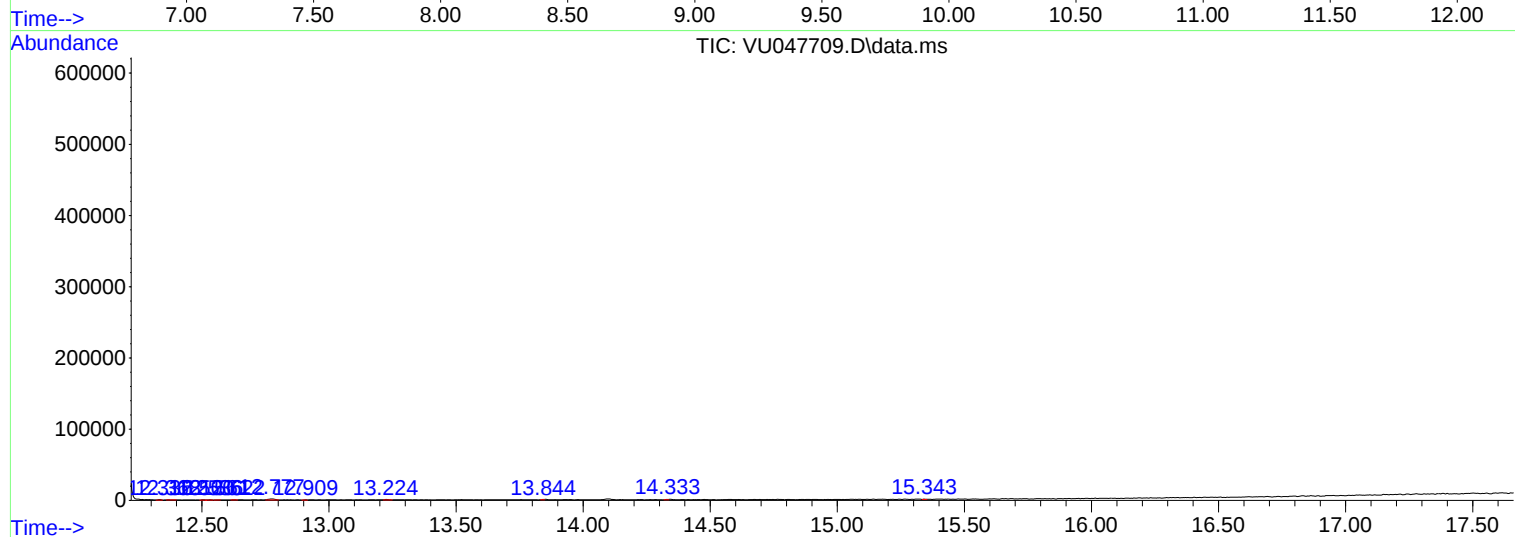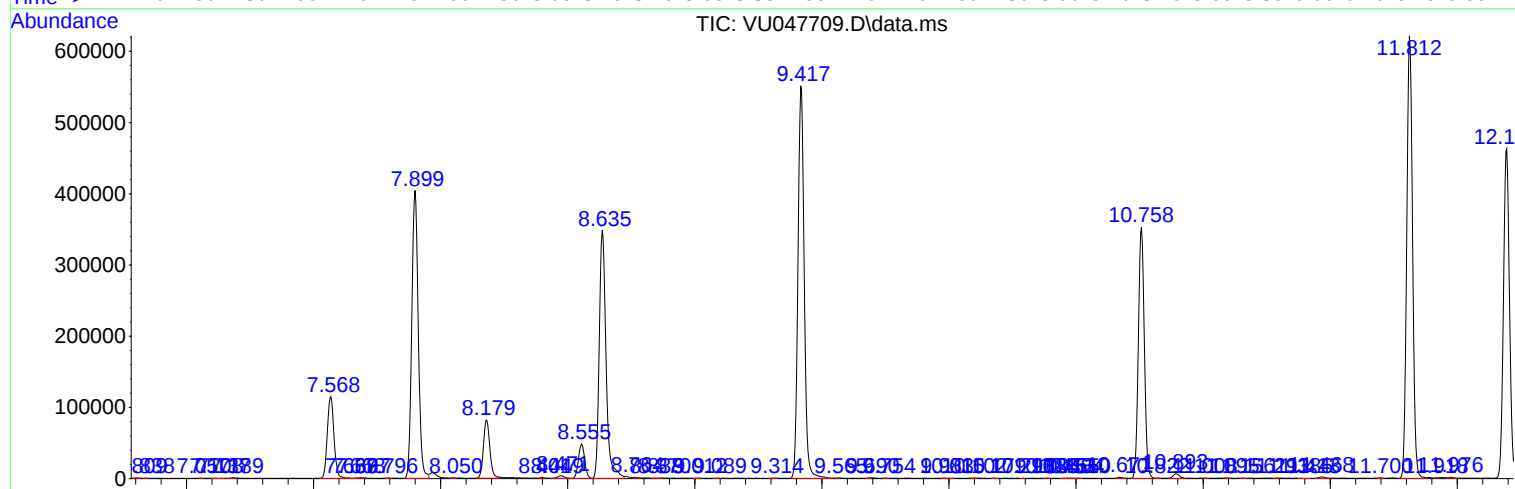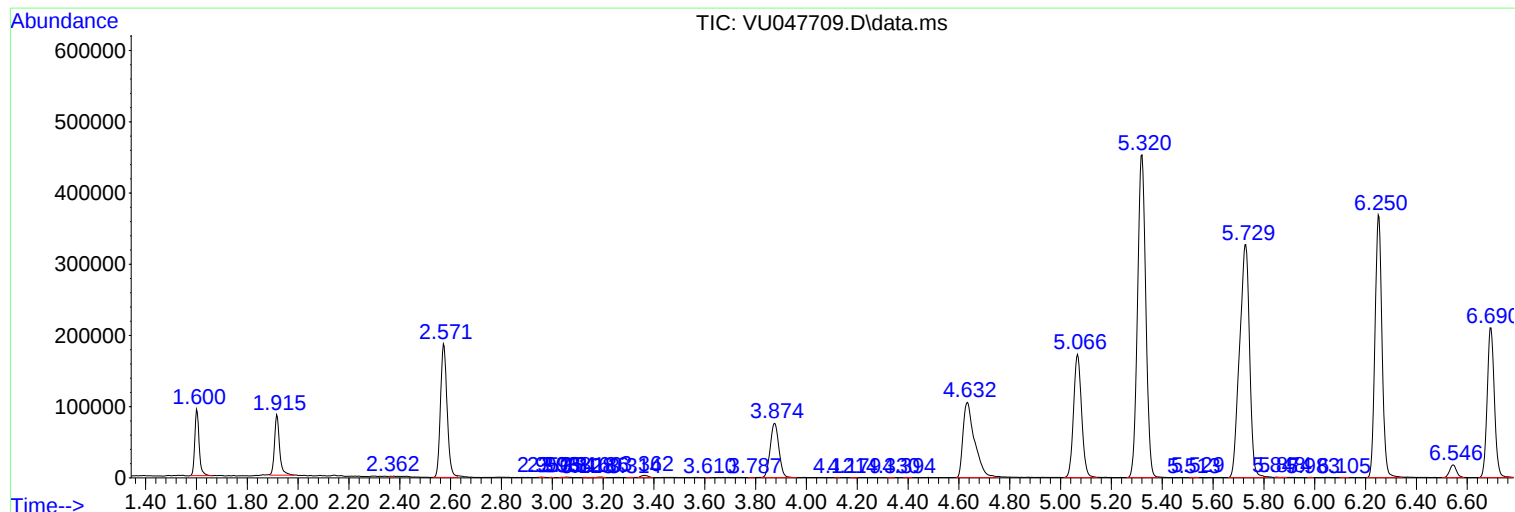

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047709.D
Acq On : 26 Mar 2022 15:19
Operator : SY/MD
Sample : N2081-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047709.D
Acq On : 26 Mar 2022 15:19
Operator : SY/MD
Sample : N2081-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5X4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------