

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047711.D
 Acq On : 26 Mar 2022 16:05
 Operator : SY/MD
 Sample : VIBLK052
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047711.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	103	rVB	133572	159232	13.41%	1.598%
2	1.919	170	180	204	rBV	108973	154265	12.99%	1.548%
3	2.572	366	383	419	rBV	238487	404646	34.07%	4.060%
4	3.051	526	532	541	rVB3	1080	1665	0.14%	0.017%
5	3.202	574	579	582	rBV	256	234	0.02%	0.002%
6	3.279	600	603	607	rVV2	323	274	0.02%	0.003%
7	3.314	607	614	620	rVB2	352	557	0.05%	0.006%
8	3.392	633	638	641	rVB2	233	260	0.02%	0.003%
9	3.427	641	649	653	rBV3	229	329	0.03%	0.003%
10	3.523	677	679	686	rVB2	319	291	0.02%	0.003%
11	3.568	690	693	695	rBV	353	243	0.02%	0.002%
12	3.752	747	750	756	rVB2	314	315	0.03%	0.003%
13	3.877	785	789	790	rBV3	385	258	0.02%	0.003%
14	3.903	795	797	803	rVV3	314	269	0.02%	0.003%
15	3.951	809	812	815	rVB2	315	241	0.02%	0.002%
16	3.980	815	821	824	rBV	383	369	0.03%	0.004%
17	3.999	824	827	832	rBV3	243	246	0.02%	0.002%
18	4.099	855	858	861	rBV3	364	242	0.02%	0.002%
19	4.642	1007	1027	1071	rVV	114156	395049	33.26%	3.963%
20	5.067	1143	1159	1182	rBV	219780	478765	40.31%	4.803%
21	5.215	1201	1205	1212	rVB3	485	509	0.04%	0.005%
22	5.263	1212	1220	1223	rBV4	377	332	0.03%	0.003%
23	5.305	1223	1233	1236	rBV3	784	1132	0.10%	0.011%
24	5.366	1246	1252	1256	rBV2	247	296	0.02%	0.003%
25	5.417	1263	1268	1273	rVB2	237	231	0.02%	0.002%
26	5.726	1343	1364	1398	rBV2	435747	1187646	100.00%	11.916%
27	6.250	1513	1527	1554	rBV	371103	701103	59.03%	7.034%
28	6.398	1570	1573	1578	rVB2	450	302	0.03%	0.003%
29	6.478	1596	1598	1602	rVB3	486	309	0.03%	0.003%
30	6.504	1602	1606	1609	rBV2	475	383	0.03%	0.004%
31	6.526	1609	1613	1615	rBV2	1385	1163	0.10%	0.012%
32	6.694	1649	1665	1688	rBV	276437	536033	45.13%	5.378%
33	6.797	1694	1697	1701	rBV3	550	488	0.04%	0.005%
34	6.816	1701	1703	1710	rVV3	502	454	0.04%	0.005%
35	7.034	1769	1771	1775	rVV3	326	273	0.02%	0.003%
36	7.057	1775	1778	1784	rVB3	529	397	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047711.D
 Acq On : 26 Mar 2022 16:05
 Operator : SY/MD
 Sample : VIBLK052
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.195	1809	1821	1831	rBV5	1927	3809	0.32%	0.038%
38	7.568	1923	1937	1960	rBV	151129	269001	22.65%	2.699%
39	7.700	1968	1978	1987	rVB7	1467	2654	0.22%	0.027%
40	7.800	2005	2009	2012	rBV2	472	461	0.04%	0.005%
41	7.899	2025	2040	2056	rBV	535389	934558	78.69%	9.376%
42	8.179	2115	2127	2151	rBV	106697	186799	15.73%	1.874%
43	8.478	2212	2220	2227	rVB4	1093	1599	0.13%	0.016%
44	8.558	2239	2245	2252	rVB4	1547	1883	0.16%	0.019%
45	8.636	2255	2269	2307	rBV	452840	850864	71.64%	8.537%
46	8.845	2330	2334	2338	rVB4	424	378	0.03%	0.004%
47	8.989	2375	2379	2385	rBV2	256	317	0.03%	0.003%
48	9.105	2412	2415	2419	rBV3	253	230	0.02%	0.002%
49	9.218	2444	2450	2454	rVB2	534	703	0.06%	0.007%
50	9.253	2454	2461	2462	rBV	358	424	0.04%	0.004%
51	9.417	2499	2512	2549	rVV	546336	922652	77.69%	9.257%
52	9.571	2553	2560	2567	rBV2	1018	1303	0.11%	0.013%
53	9.697	2586	2599	2600	rBV5	1300	1693	0.14%	0.017%
54	9.774	2618	2623	2627	rVB	284	247	0.02%	0.002%
55	9.861	2646	2650	2652	rBV2	244	226	0.02%	0.002%
56	10.034	2699	2704	2710	rVB2	318	446	0.04%	0.004%
57	10.099	2721	2724	2729	rBV3	474	487	0.04%	0.005%
58	10.205	2754	2757	2759	rVB3	369	239	0.02%	0.002%
59	10.227	2759	2764	2767	rBV	240	261	0.02%	0.003%
60	10.301	2783	2787	2789	rBV2	298	230	0.02%	0.002%
61	10.372	2801	2809	2812	rBV2	229	367	0.03%	0.004%
62	10.427	2821	2826	2829	rBV	277	271	0.02%	0.003%
63	10.481	2838	2843	2846	rBV	546	495	0.04%	0.005%
64	10.668	2896	2901	2902	rBV3	797	610	0.05%	0.006%
65	10.758	2916	2929	2948	rBV	442970	713145	60.05%	7.155%
66	10.899	2963	2973	2987	rVB5	2545	4885	0.41%	0.049%
67	10.999	2998	3004	3005	rBV	1143	998	0.08%	0.010%
68	11.092	3025	3033	3041	rVB3	2911	4179	0.35%	0.042%
69	11.295	3088	3096	3106	rVB5	3303	4962	0.42%	0.050%
70	11.468	3139	3150	3162	rBV3	19095	29212	2.46%	0.293%
71	11.745	3231	3236	3243	rVB4	749	1022	0.09%	0.010%
72	11.812	3243	3257	3274	rBV	620261	988162	83.20%	9.914%
73	11.896	3277	3283	3291	rVB3	5697	8293	0.70%	0.083%
74	11.970	3303	3306	3315	rVB5	1309	1600	0.13%	0.016%
75	12.015	3315	3320	3322	rBV4	405	358	0.03%	0.004%
76	12.095	3338	3345	3351	rBV5	2178	3202	0.27%	0.032%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047711.D
 Acq On : 26 Mar 2022 16:05
 Operator : SY/MD
 Sample : VIBLK052
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	12.192	3362	3375	3392	rBV	590929	954556	80.37%	9.577%
78	12.285	3402	3404	3411	rVB3	490	503	0.04%	0.005%
79	12.381	3426	3434	3440	rBV5	809	1226	0.10%	0.012%
80	12.494	3451	3469	3479	rBV10	2426	5678	0.48%	0.057%
81	12.571	3487	3493	3503	rVB4	1869	2692	0.23%	0.027%
82	12.623	3506	3509	3513	rBV	317	226	0.02%	0.002%
83	12.671	3522	3524	3526	rBV	384	222	0.02%	0.002%
84	12.777	3550	3557	3562	rVB4	764	1074	0.09%	0.011%
85	12.806	3562	3566	3570	rBV3	292	263	0.02%	0.003%
86	12.883	3584	3590	3599	rVB5	724	982	0.08%	0.010%
87	12.973	3615	3618	3619	rBV2	473	300	0.03%	0.003%
88	13.034	3631	3637	3642	rVB3	1401	1727	0.15%	0.017%
89	13.298	3712	3719	3723	rBV3	586	834	0.07%	0.008%
90	13.359	3734	3738	3741	rBV3	272	222	0.02%	0.002%
91	13.378	3741	3744	3747	rVV3	433	323	0.03%	0.003%
92	13.449	3761	3766	3780	rVB5	2101	3034	0.26%	0.030%
93	13.838	3883	3887	3888	rBV3	766	551	0.05%	0.006%
94	14.089	3957	3965	3977	rVB2	10199	16521	1.39%	0.166%
95	14.359	4046	4049	4051	rBV2	330	253	0.02%	0.003%
96	14.565	4111	4113	4117	rVB2	459	214	0.02%	0.002%
97	15.227	4312	4319	4320	rBV5	1930	1793	0.15%	0.018%
98	15.327	4348	4350	4353	rBV	512	397	0.03%	0.004%
99	15.369	4360	4363	4368	rBV4	486	460	0.04%	0.005%
100	15.880	4518	4522	4526	rBV4	1025	1150	0.10%	0.012%




Sum of corrected areas: 9967227

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047711.D
Acq On : 26 Mar 2022 16:05
Operator : SY/MD
Sample : VIBLK052
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

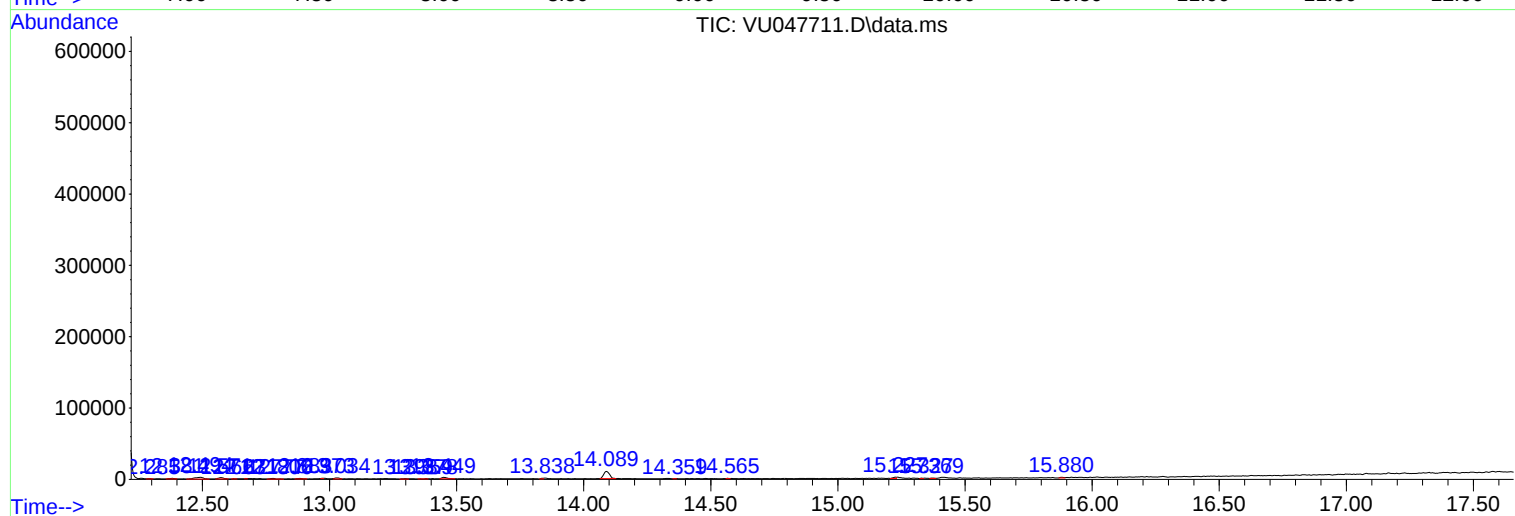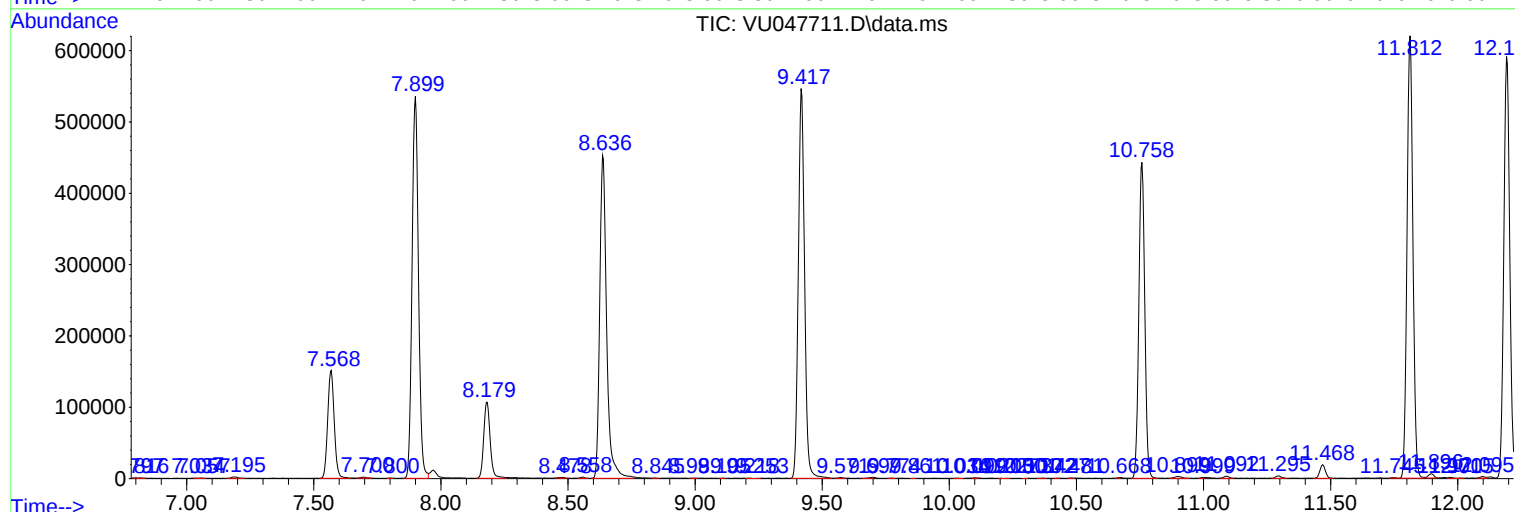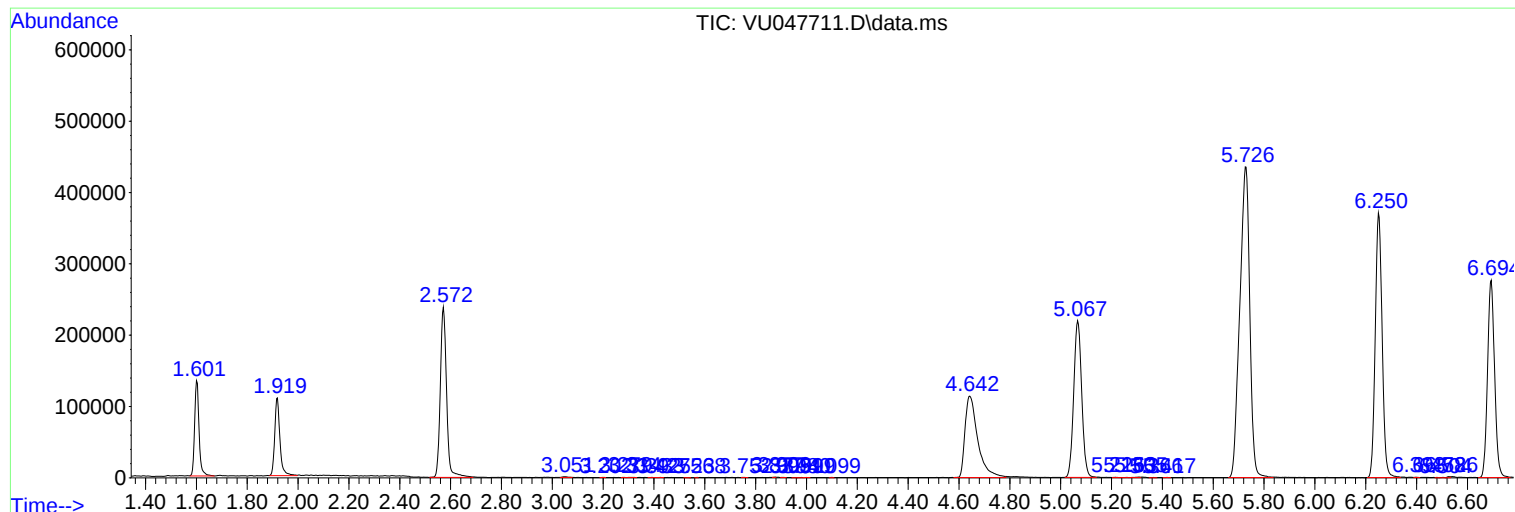

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047711.D
Acq On : 26 Mar 2022 16:05
Operator : SY/MD
Sample : VIBLK052
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047711.D
Acq On : 26 Mar 2022 16:05
Operator : SY/MD
Sample : VIBLK052
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------