

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047715.D
 Acq On : 26 Mar 2022 17:36
 Operator : SY/MD
 Sample : N2081-15DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU047715.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	100	rBV	135167	165702	14.04%	1.398%
2	1.919	170	180	183	rBV	121710	161880	13.72%	1.366%
3	2.517	364	366	370	rVB2	340	237	0.02%	0.002%
4	2.571	370	383	409	rBV	235853	408285	34.60%	3.446%
5	2.800	444	454	461	rBV3	1253	1934	0.16%	0.016%
6	3.057	524	534	541	rVB5	1316	2190	0.19%	0.018%
7	3.186	568	574	578	rBV3	616	894	0.08%	0.008%
8	3.359	617	628	638	rBV5	2969	5714	0.48%	0.048%
9	3.658	716	721	725	rBV3	230	246	0.02%	0.002%
10	3.745	744	748	751	rBV2	306	251	0.02%	0.002%
11	3.806	764	767	771	rVB2	311	223	0.02%	0.002%
12	3.874	771	788	811	rBV2	108892	261944	22.20%	2.211%
13	3.954	811	813	817	rVV2	426	272	0.02%	0.002%
14	3.983	819	822	826	rVB2	534	433	0.04%	0.004%
15	4.063	843	847	850	rBV2	302	250	0.02%	0.002%
16	4.349	933	936	942	rBV2	283	289	0.02%	0.002%
17	4.668	1010	1035	1055	rBV3	223034	807109	68.41%	6.812%
18	5.066	1143	1159	1187	rVV	216432	473443	40.13%	3.996%
19	5.320	1219	1238	1257	rVV	359405	814184	69.01%	6.871%
20	5.459	1279	1281	1288	rVB3	432	432	0.04%	0.004%
21	5.491	1288	1291	1293	rBV2	475	290	0.02%	0.002%
22	5.536	1303	1305	1310	rVB3	412	263	0.02%	0.002%
23	5.581	1315	1319	1321	rBV3	278	224	0.02%	0.002%
24	5.726	1341	1364	1393	rBV2	435397	1179852	100.00%	9.957%
25	6.015	1449	1454	1458	rBV4	282	294	0.02%	0.002%
26	6.038	1458	1461	1468	rVB3	480	419	0.04%	0.004%
27	6.250	1512	1527	1549	rBV	381334	723072	61.28%	6.102%
28	6.452	1588	1590	1597	rVB3	351	380	0.03%	0.003%
29	6.542	1609	1618	1632	rBV5	6700	12828	1.09%	0.108%
30	6.629	1642	1645	1647	rBV2	434	225	0.02%	0.002%
31	6.693	1650	1665	1684	rBV	271821	529469	44.88%	4.468%
32	6.915	1728	1734	1737	rBV	167	225	0.02%	0.002%
33	7.028	1765	1769	1772	rBV2	299	274	0.02%	0.002%
34	7.182	1810	1817	1826	rBV5	2330	4501	0.38%	0.038%
35	7.269	1839	1844	1847	rVB3	233	240	0.02%	0.002%
36	7.343	1863	1867	1871	rVB3	330	297	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047715.D
 Acq On : 26 Mar 2022 17:36
 Operator : SY/MD
 Sample : N2081-15DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.369	1871	1875	1883	rBV3	240	270	0.02%	0.002%
38	7.427	1888	1893	1896	rBV2	220	219	0.02%	0.002%
39	7.568	1924	1937	1962	rVV	151939	267619	22.68%	2.259%
40	7.661	1962	1966	1968	rBV3	423	369	0.03%	0.003%
41	7.690	1968	1975	1982	rVB4	1419	2159	0.18%	0.018%
42	7.793	2000	2007	2016	rBV4	2349	3620	0.31%	0.031%
43	7.899	2026	2040	2054	rBV	533969	932116	79.00%	7.867%
44	7.970	2056	2062	2079	rVB	34851	59300	5.03%	0.500%
45	8.179	2115	2127	2150	rBV	106234	186120	15.77%	1.571%
46	8.407	2195	2198	2201	rVB3	333	229	0.02%	0.002%
47	8.471	2210	2218	2230	rVB3	5170	9399	0.80%	0.079%
48	8.523	2230	2234	2235	rBV2	316	232	0.02%	0.002%
49	8.552	2235	2243	2255	rVB3	14945	24398	2.07%	0.206%
50	8.635	2256	2269	2304	rBV	468703	876172	74.26%	7.394%
51	8.783	2313	2315	2318	rVB2	720	426	0.04%	0.004%
52	8.803	2318	2321	2324	rBV3	483	310	0.03%	0.003%
53	8.880	2341	2345	2351	rBV3	366	401	0.03%	0.003%
54	8.925	2356	2359	2367	rVB3	518	619	0.05%	0.005%
55	9.021	2387	2389	2396	rBV2	232	216	0.02%	0.002%
56	9.362	2491	2495	2499	rVB3	246	226	0.02%	0.002%
57	9.417	2499	2512	2542	rBV	563943	950001	80.52%	8.017%
58	9.571	2550	2560	2573	rVB2	8243	13195	1.12%	0.111%
59	9.693	2587	2598	2613	rBV	17989	29017	2.46%	0.245%
60	9.944	2673	2676	2678	rBV2	351	265	0.02%	0.002%
61	10.015	2694	2698	2702	rVB	315	276	0.02%	0.002%
62	10.057	2708	2711	2716	rVB2	296	227	0.02%	0.002%
63	10.102	2716	2725	2737	rBV	11842	19659	1.67%	0.166%
64	10.172	2741	2747	2750	rBV2	244	270	0.02%	0.002%
65	10.295	2782	2785	2793	rVB3	314	291	0.02%	0.002%
66	10.340	2793	2799	2803	rBV3	234	222	0.02%	0.002%
67	10.385	2810	2813	2817	rVB3	278	223	0.02%	0.002%
68	10.484	2836	2844	2853	rVB	2167	2914	0.25%	0.025%
69	10.671	2890	2902	2910	rBV6	1248	2015	0.17%	0.017%
70	10.758	2915	2929	2948	rVV	444973	719777	61.01%	6.074%
71	10.825	2948	2950	2959	rVV5	1300	1351	0.11%	0.011%
72	10.896	2961	2972	2983	rVB3	9628	17382	1.47%	0.147%
73	10.999	2995	3004	3010	rBV2	7351	11995	1.02%	0.101%
74	11.092	3025	3033	3043	rVB2	5058	7306	0.62%	0.062%
75	11.240	3076	3079	3082	rBV2	385	234	0.02%	0.002%
76	11.291	3087	3095	3108	rVB	6951	10311	0.87%	0.087%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047715.D
 Acq On : 26 Mar 2022 17:36
 Operator : SY/MD
 Sample : N2081-15DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.417	3130	3134	3136	rBV2	328	270	0.02%	0.002%
78	11.468	3140	3150	3161	rVB	25961	38598	3.27%	0.326%
79	11.565	3177	3180	3182	rBV2	360	228	0.02%	0.002%
80	11.680	3213	3216	3217	rBV	345	223	0.02%	0.002%
81	11.693	3217	3220	3222	rVV2	343	279	0.02%	0.002%
82	11.748	3230	3237	3244	rBV7	3133	4813	0.41%	0.041%
83	11.812	3244	3257	3274	rVV	651285	1028600	87.18%	8.681%
84	11.893	3274	3282	3292	rVB2	11297	17134	1.45%	0.145%
85	11.973	3302	3307	3315	rVB4	1084	1304	0.11%	0.011%
86	12.098	3336	3346	3351	rBV2	4939	7037	0.60%	0.059%
87	12.195	3361	3376	3393	rBV	595631	974038	82.56%	8.220%
88	12.378	3425	3433	3438	rBV	1124	1265	0.11%	0.011%
89	12.471	3454	3462	3464	rBV2	1343	1579	0.13%	0.013%
90	12.491	3465	3468	3478	rVB7	1774	2263	0.19%	0.019%
91	12.574	3488	3494	3500	rBV3	1271	1517	0.13%	0.013%
92	12.774	3547	3556	3564	rVB4	2836	4673	0.40%	0.039%
93	13.224	3687	3696	3705	rBV4	2822	4596	0.39%	0.039%
94	13.449	3761	3766	3773	rVB5	1423	1975	0.17%	0.017%
95	13.552	3795	3798	3802	rBV2	280	264	0.02%	0.002%
96	13.622	3818	3820	3827	rVB2	315	245	0.02%	0.002%
97	13.847	3881	3890	3898	rVB3	5080	7494	0.64%	0.063%
98	14.089	3956	3965	3985	rVB2	18639	31090	2.64%	0.262%
99	14.243	4010	4013	4016	rBV3	334	285	0.02%	0.002%
100	14.330	4033	4040	4049	rBV2	6652	9271	0.79%	0.078%


Sum of corrected areas: 11849157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047715.D
Acq On : 26 Mar 2022 17:36
Operator : SY/MD
Sample : N2081-15DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

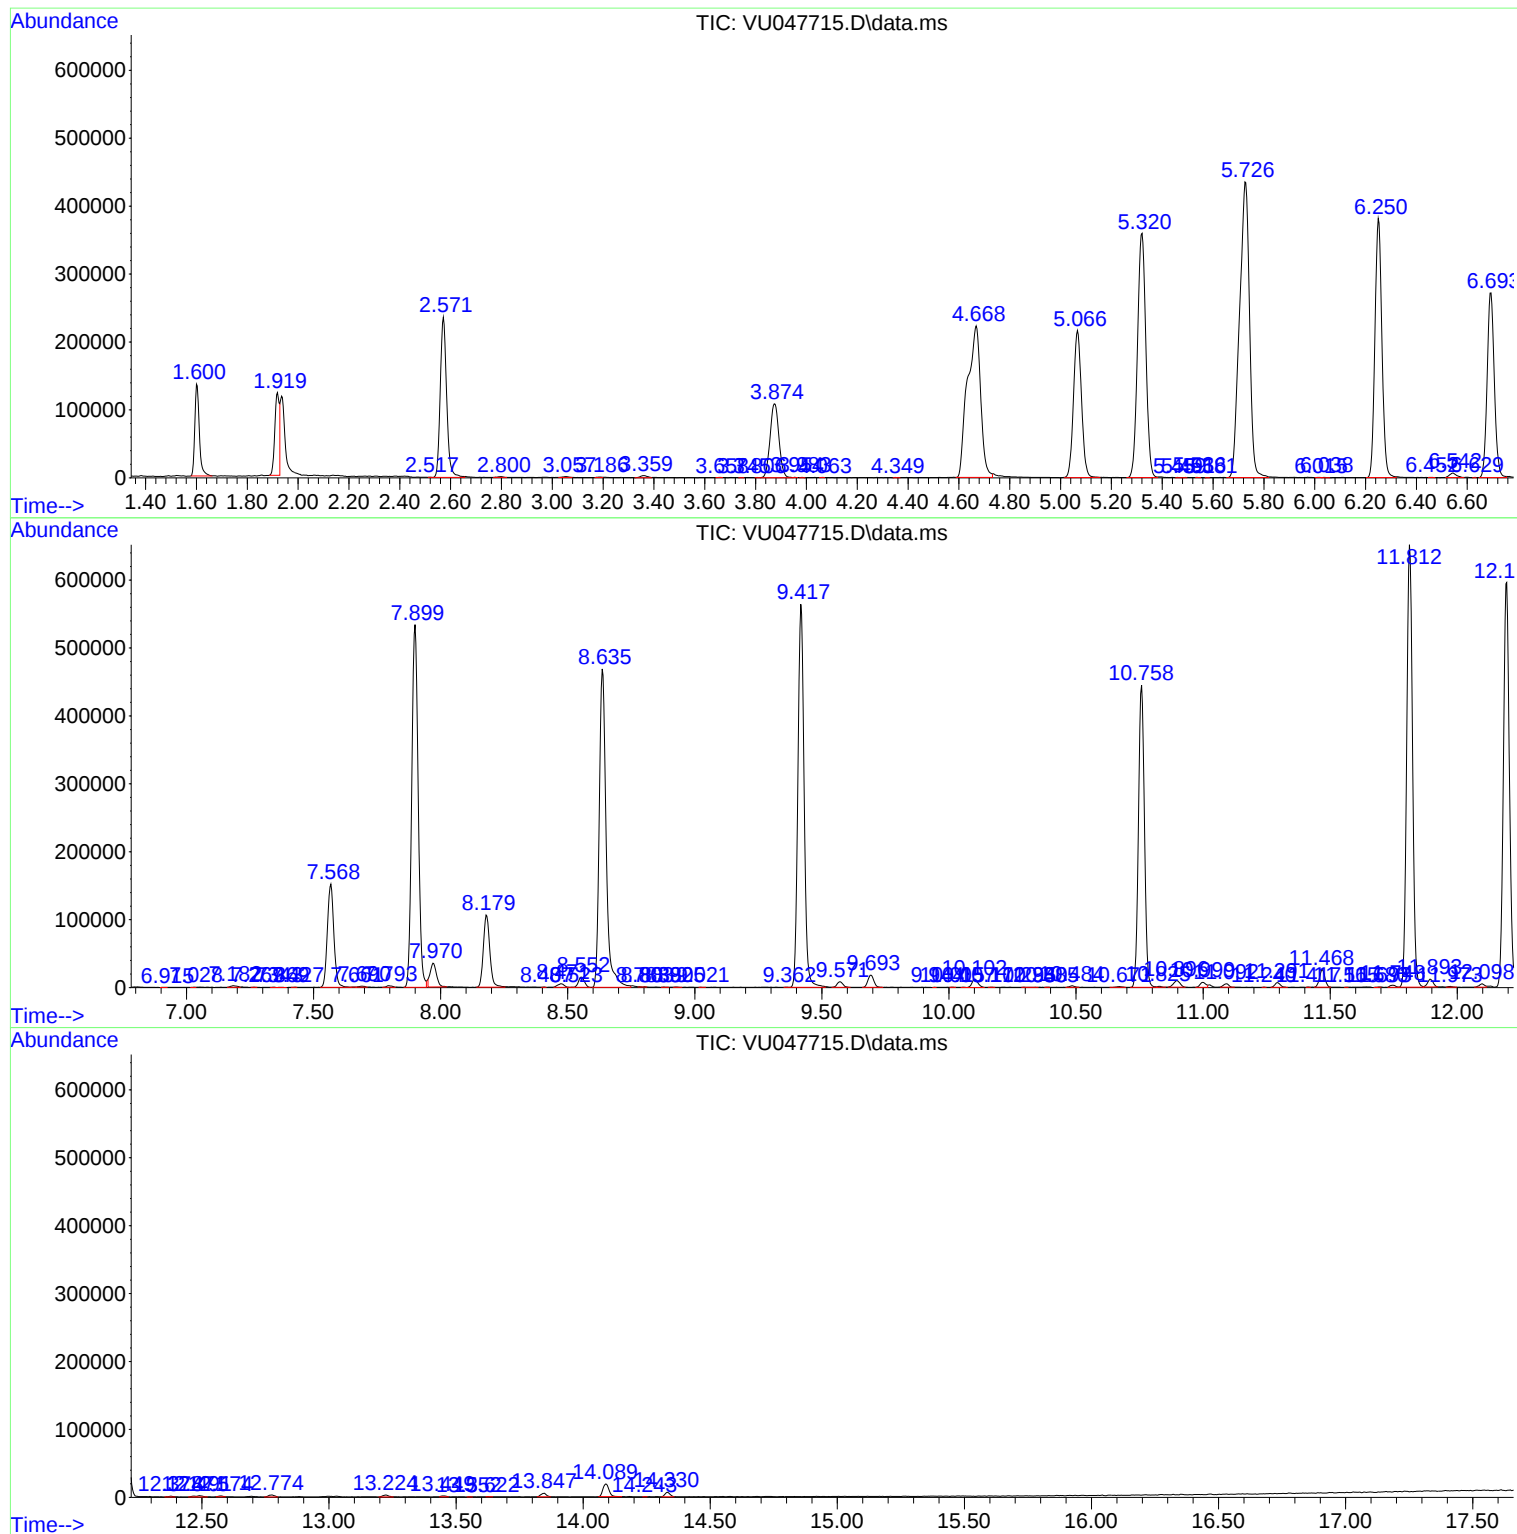

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047715.D
Acq On : 26 Mar 2022 17:36
Operator : SY/MD
Sample : N2081-15DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047715.D
Acq On : 26 Mar 2022 17:36
Operator : SY/MD
Sample : N2081-15DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------