

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047717.D
 Acq On : 26 Mar 2022 18:21
 Operator : SY/MD
 Sample : N2081-18DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU047717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	98	rBV	129993	152101	12.93%	1.541%
2	1.916	170	179	206	rVB	116620	165330	14.06%	1.675%
3	2.571	370	383	410	rBV	234597	395160	33.59%	4.004%
4	2.700	420	423	429	rVB4	430	376	0.03%	0.004%
5	2.787	447	450	451	rBV2	308	204	0.02%	0.002%
6	2.800	451	454	460	rVB3	810	871	0.07%	0.009%
7	3.006	511	518	521	rBV2	280	301	0.03%	0.003%
8	3.047	525	531	541	rBV3	1286	2246	0.19%	0.023%
9	3.485	664	667	671	rVB2	344	263	0.02%	0.003%
10	3.507	671	674	678	rBV2	352	310	0.03%	0.003%
11	3.883	789	791	796	rVB3	389	236	0.02%	0.002%
12	3.915	796	801	807	rBV	279	341	0.03%	0.003%
13	4.128	864	867	871	rVB	323	239	0.02%	0.002%
14	4.308	921	923	928	rVB3	272	211	0.02%	0.002%
15	4.504	981	984	988	rBV3	403	333	0.03%	0.003%
16	4.629	1010	1023	1051	rBV	138926	367490	31.24%	3.724%
17	4.906	1106	1109	1113	rVB2	359	231	0.02%	0.002%
18	4.932	1114	1117	1121	rVB2	339	230	0.02%	0.002%
19	5.067	1141	1159	1189	rBV	215002	470257	39.98%	4.765%
20	5.292	1224	1229	1234	rVV3	453	611	0.05%	0.006%
21	5.729	1343	1365	1396	rBV2	431506	1176269	100.00%	11.920%
22	5.989	1443	1446	1448	rBV	266	206	0.02%	0.002%
23	6.038	1457	1461	1464	rBV3	352	309	0.03%	0.003%
24	6.083	1468	1475	1480	rBV2	444	425	0.04%	0.004%
25	6.112	1480	1484	1490	rBV2	297	369	0.03%	0.004%
26	6.173	1500	1503	1508	rVB2	255	243	0.02%	0.002%
27	6.250	1508	1527	1549	rBV	375161	710954	60.44%	7.205%
28	6.446	1582	1588	1592	rVB3	316	309	0.03%	0.003%
29	6.510	1603	1608	1609	rBV3	399	324	0.03%	0.003%
30	6.530	1609	1614	1618	rBV6	1332	1752	0.15%	0.018%
31	6.693	1651	1665	1683	rBV	273821	534575	45.45%	5.417%
32	6.771	1687	1689	1695	rVV4	944	821	0.07%	0.008%
33	6.800	1695	1698	1705	rVB5	427	515	0.04%	0.005%
34	6.989	1753	1757	1762	rBV3	200	217	0.02%	0.002%
35	7.047	1769	1775	1778	rBV	384	409	0.03%	0.004%
36	7.115	1792	1796	1802	rBV3	418	387	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047717.D
 Acq On : 26 Mar 2022 18:21
 Operator : SY/MD
 Sample : N2081-18DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.147	1803	1806	1810	rVB2	390	253	0.02%	0.003%
38	7.189	1810	1819	1829	rBV5	2363	4361	0.37%	0.044%
39	7.385	1874	1880	1883	rBV3	345	389	0.03%	0.004%
40	7.446	1896	1899	1904	rBV2	332	343	0.03%	0.003%
41	7.484	1904	1911	1915	rBV2	387	459	0.04%	0.005%
42	7.568	1923	1937	1958	rBV	147368	264084	22.45%	2.676%
43	7.690	1970	1975	1980	rVB5	1261	1574	0.13%	0.016%
44	7.793	2002	2007	2016	rBV5	821	1137	0.10%	0.012%
45	7.899	2025	2040	2056	rBV	537261	934503	79.45%	9.470%
46	8.121	2103	2109	2114	rBV2	245	289	0.02%	0.003%
47	8.179	2114	2127	2142	rBV	105193	180797	15.37%	1.832%
48	8.472	2210	2218	2225	rBV	1172	1806	0.15%	0.018%
49	8.555	2239	2244	2247	rBV4	768	570	0.05%	0.006%
50	8.636	2254	2269	2300	rBV	462912	852153	72.45%	8.635%
51	8.851	2334	2336	2338	rBV2	373	232	0.02%	0.002%
52	8.886	2344	2347	2349	rBV2	526	367	0.03%	0.004%
53	9.163	2427	2433	2435	rBV3	270	308	0.03%	0.003%
54	9.346	2484	2490	2493	rBV3	239	236	0.02%	0.002%
55	9.417	2497	2512	2547	rBV	553886	940368	79.94%	9.529%
56	9.571	2555	2560	2566	rVB2	820	822	0.07%	0.008%
57	9.697	2590	2599	2609	rVB5	1265	2159	0.18%	0.022%
58	9.767	2617	2621	2624	rBV2	397	323	0.03%	0.003%
59	9.793	2626	2629	2634	rVB3	292	288	0.02%	0.003%
60	9.832	2637	2641	2642	rBV	386	246	0.02%	0.002%
61	9.989	2687	2690	2695	rVB3	313	253	0.02%	0.003%
62	10.102	2718	2725	2726	rBV3	869	835	0.07%	0.008%
63	10.436	2826	2829	2833	rBV2	279	291	0.02%	0.003%
64	10.488	2836	2845	2848	rVV3	454	605	0.05%	0.006%
65	10.668	2896	2901	2908	rVV4	1391	1573	0.13%	0.016%
66	10.758	2915	2929	2946	rBV	433272	706623	60.07%	7.161%
67	10.835	2950	2953	2956	rVB	440	293	0.02%	0.003%
68	10.896	2962	2972	2982	rBV5	2176	3773	0.32%	0.038%
69	10.973	2993	2996	2999	rBV	255	215	0.02%	0.002%
70	10.996	2999	3003	3005	rVV	364	304	0.03%	0.003%
71	11.015	3006	3009	3013	rVB2	336	284	0.02%	0.003%
72	11.089	3026	3032	3040	rBV3	949	1441	0.12%	0.015%
73	11.121	3040	3042	3047	rVB3	330	218	0.02%	0.002%
74	11.172	3053	3058	3061	rBV	222	205	0.02%	0.002%
75	11.282	3087	3092	3093	rBV2	347	224	0.02%	0.002%
76	11.295	3093	3096	3100	rBV3	456	432	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
 Data File : VU047717.D
 Acq On : 26 Mar 2022 18:21
 Operator : SY/MD
 Sample : N2081-18DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5Y5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.471	3141	3151	3161	rVB3	5664	9127	0.78%	0.092%
78	11.516	3162	3165	3171	rBV2	286	268	0.02%	0.003%
79	11.571	3179	3182	3187	rBV	322	204	0.02%	0.002%
80	11.751	3231	3238	3243	rVB4	642	791	0.07%	0.008%
81	11.812	3244	3257	3277	rBV	637930	997797	84.83%	10.111%
82	11.925	3289	3292	3294	rBV2	386	226	0.02%	0.002%
83	12.005	3314	3317	3322	rVB2	342	301	0.03%	0.003%
84	12.098	3341	3346	3350	rVB4	540	493	0.04%	0.005%
85	12.192	3362	3375	3393	rBV	587158	947347	80.54%	9.600%
86	12.291	3404	3406	3412	rVB5	512	472	0.04%	0.005%
87	12.323	3412	3416	3418	rBV2	328	300	0.03%	0.003%
88	12.391	3433	3437	3438	rBV2	339	205	0.02%	0.002%
89	12.439	3448	3452	3453	rBV2	267	215	0.02%	0.002%
90	12.494	3465	3469	3472	rBV4	650	609	0.05%	0.006%
91	12.774	3553	3556	3563	rVB3	558	556	0.05%	0.006%
92	13.224	3690	3696	3707	rVB4	1161	1780	0.15%	0.018%
93	13.455	3762	3768	3772	rBV3	657	867	0.07%	0.009%
94	13.500	3779	3782	3788	rBV3	285	352	0.03%	0.004%
95	13.844	3884	3889	3897	rVB4	1897	2217	0.19%	0.022%
96	14.060	3952	3956	3957	rBV3	351	252	0.02%	0.003%
97	14.092	3957	3966	3978	rVV	5775	9586	0.81%	0.097%
98	14.336	4036	4042	4049	rVB4	1933	2331	0.20%	0.024%
99	14.565	4109	4113	4117	rBV3	332	314	0.03%	0.003%
100	14.986	4242	4244	4249	rBV3	423	417	0.04%	0.004%




Sum of corrected areas: 9868088

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047717.D
Acq On : 26 Mar 2022 18:21
Operator : SY/MD
Sample : N2081-18DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

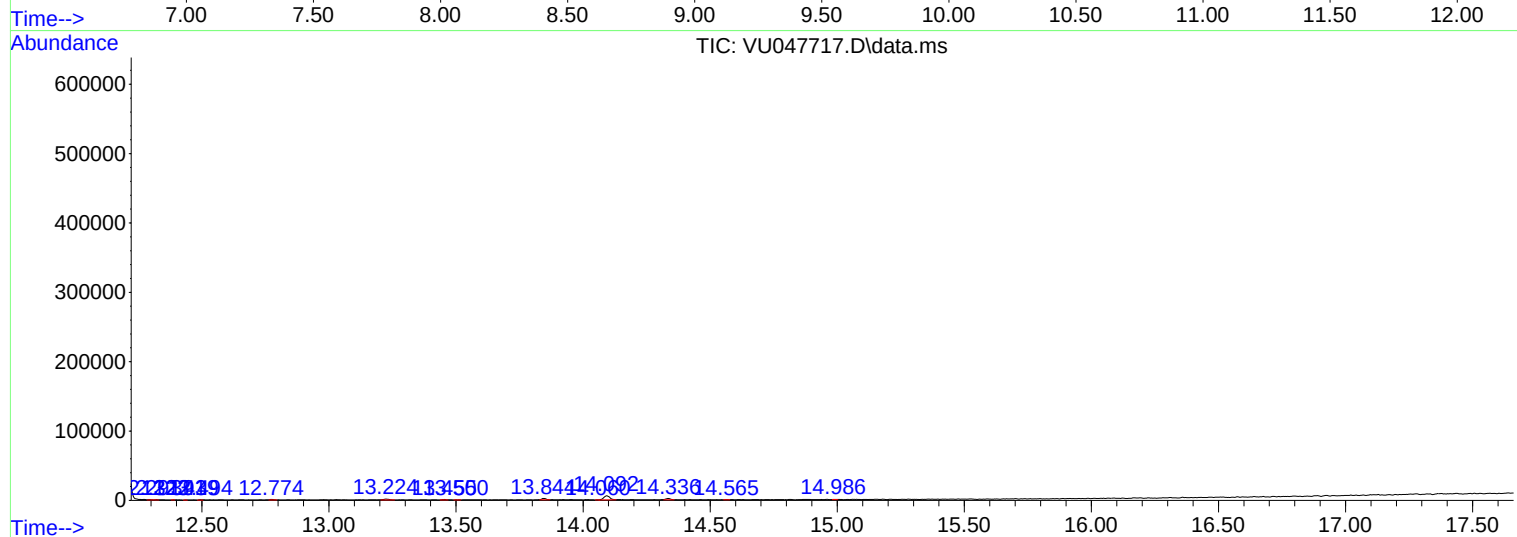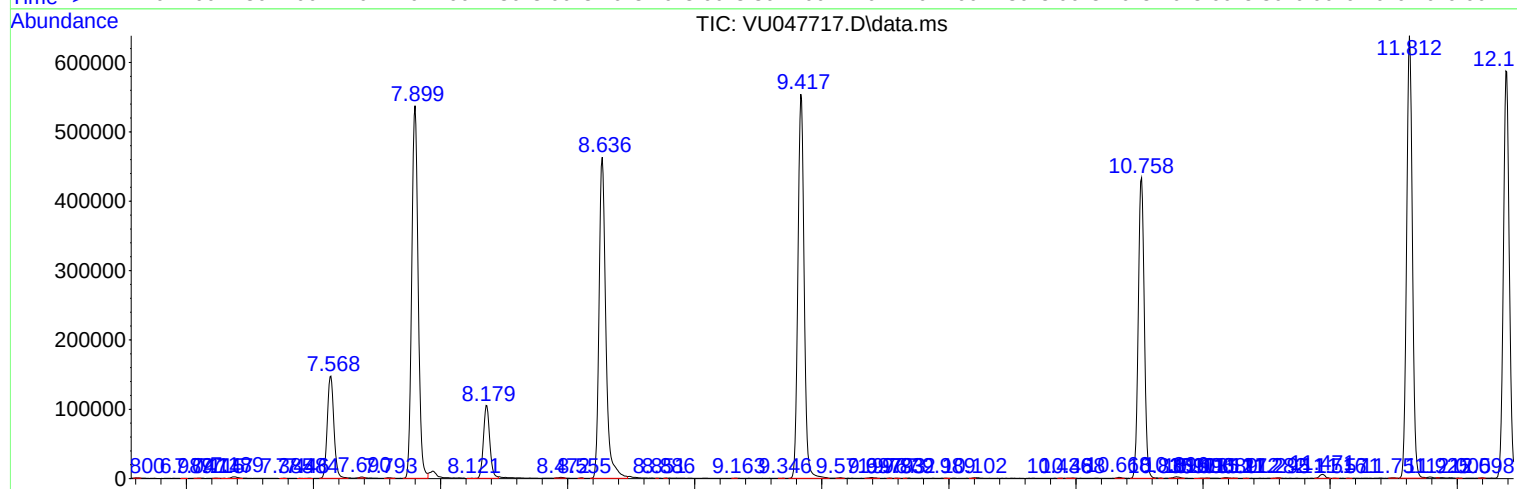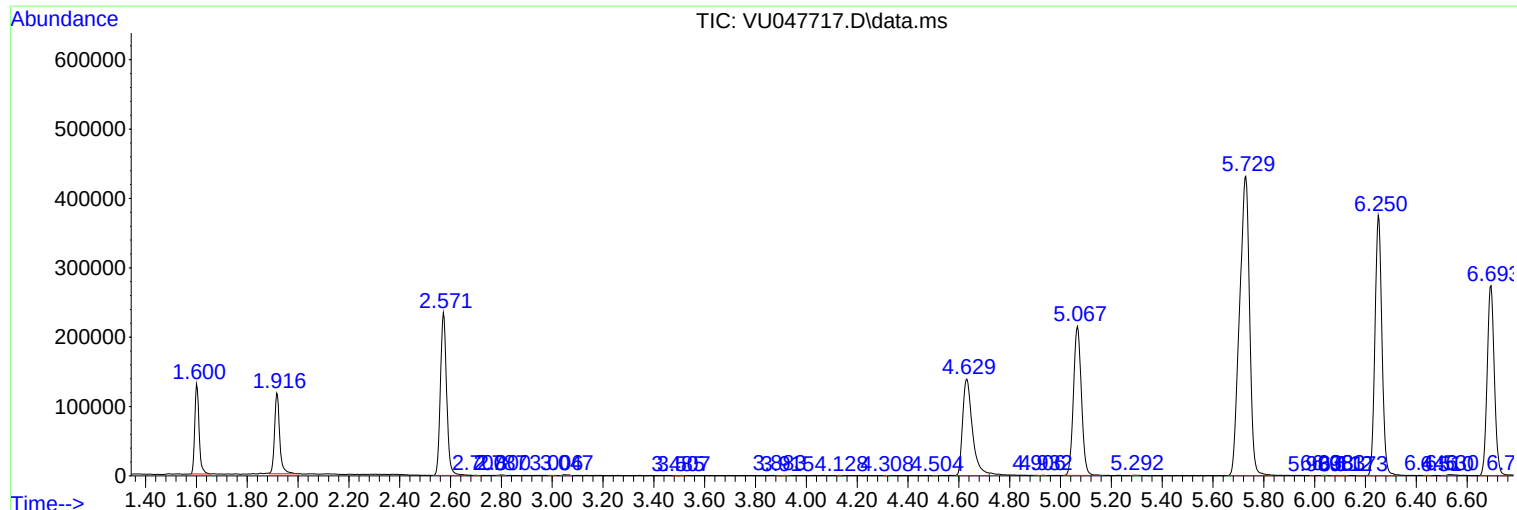

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047717.D
Acq On : 26 Mar 2022 18:21
Operator : SY/MD
Sample : N2081-18DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032622\
Data File : VU047717.D
Acq On : 26 Mar 2022 18:21
Operator : SY/MD
Sample : N2081-18DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5Y5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------